

Municipality: LONGPORT BORO Alcotest Ser.#: ARXA-0067

ALCOTEST CHECKLIST

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDXC S3-0154
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.  
Ser. #: DDWA P2-177
- 4. **Digital Temperature Measuring System Report of Calibration.**
- 5.
  - A. Alcotest 7110 Calibration Record
  - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
  - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
  - D. **Alcotest Card** of operator/coordinator who performed tests.
  - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDWA P2-016
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
  - A. 0.04% Solution. 07 A 041
  - B. 0.08% Solution. 07 A 042
  - C. 0.10% Solution. 07 B 045
  - D. 0.16% Solution. 07 A 043
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
  - A. 0.04% used in Calibration/Linearity Testing. DDWE S3-0196
  - B. 0.08% used in Calibration/Linearity Testing. DDWE S3-0203
  - C. 0.10% used in Calibration/Linearity Testing DDXC-S3-0154 [Same as instrument's CU34 unit].
  - D. 0.16% used in Calibration/Linearity Testing. DDWE S3-0205
- 8.
  - A. New Standard Solution Report - following Calibration.
  - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
  - C. Certificate of Analysis 0.10% solution for same.  
Lot #: 08 B 050
  - D. Alcotest card of operator/coordinator who completed change.

Dräger safety

Alcotest<sup>®</sup> 7110 MKIII-C

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


03/09/2000

SERIAL NUMBER:

ARXA-0067

Draeger Safety Diagnostics, Inc.  
Durango, CO

Ant D



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXC 53-0154

Certification Date

Technician

Re-Certification Due Date

JAN. 22/2008

TS

JAN. 22/2009

## Dräger safety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAP2-177

01-22-08

01-22-09

Probe Value

104

Draeger Safety Diagnostics, Inc.  
Technical Service Department

## Ertco-Hart Digital Temperature Measuring System

### REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature

verification Serial Number: HH41301316 / HH41303176 / MERCURY THERMOMETER

Digital Units Serial Number: A23730

Probe Serial Number: 773623

Certification Date: 02-13-08

Next Certification Due: 02-13-09

At 34.00 °C digital unit displays 34.07 °C

Draeger Safety Diagnostics, Inc. Technician: AE

# Alcotest 7110 Calibration Record

**Equipment** Alcotest 7110 MKIII-C  
Location: LONGPORT POLICE  
Calibration File No.: 00256  
Certification File No.: 00212  
Linearity File No.: 00213  
Solution File No.: 00247  
Sequential File No.: 00256

Serial No.: ARXA-0067  
Calib. Date: 08/26/2008  
Cert. Date: 03/28/2008  
Lin. Date: 03/28/2008  
Soln. Date: 08/15/2008  
File Date: 08/26/2008  
Calib. No.: 00005  
Cert. No.: 00003  
Lin. No.: 00003  
Soln. No.: 00052

Calibrating Unit: WET  
Control Solution %: 0.100%  
Solution Control Lot: 07B045

Model No.: CU-34  
Serial No.: DDXC S3-0154  
Expires: 02/22/2009  
Bottle No.: 0563

## Coordinator

Last Name: DELLANOCE

First Name: JOSEPH


MI: S

Signature: Joseph Dellanoce #6027

Badge No.: 6027  
Date: 08/26/2008

\*Black Key Temperature Probe Serial .....# DDWAP2-016 050

\*Ertco-Hart Digital Temperature Measuring System Serial# A23730 050

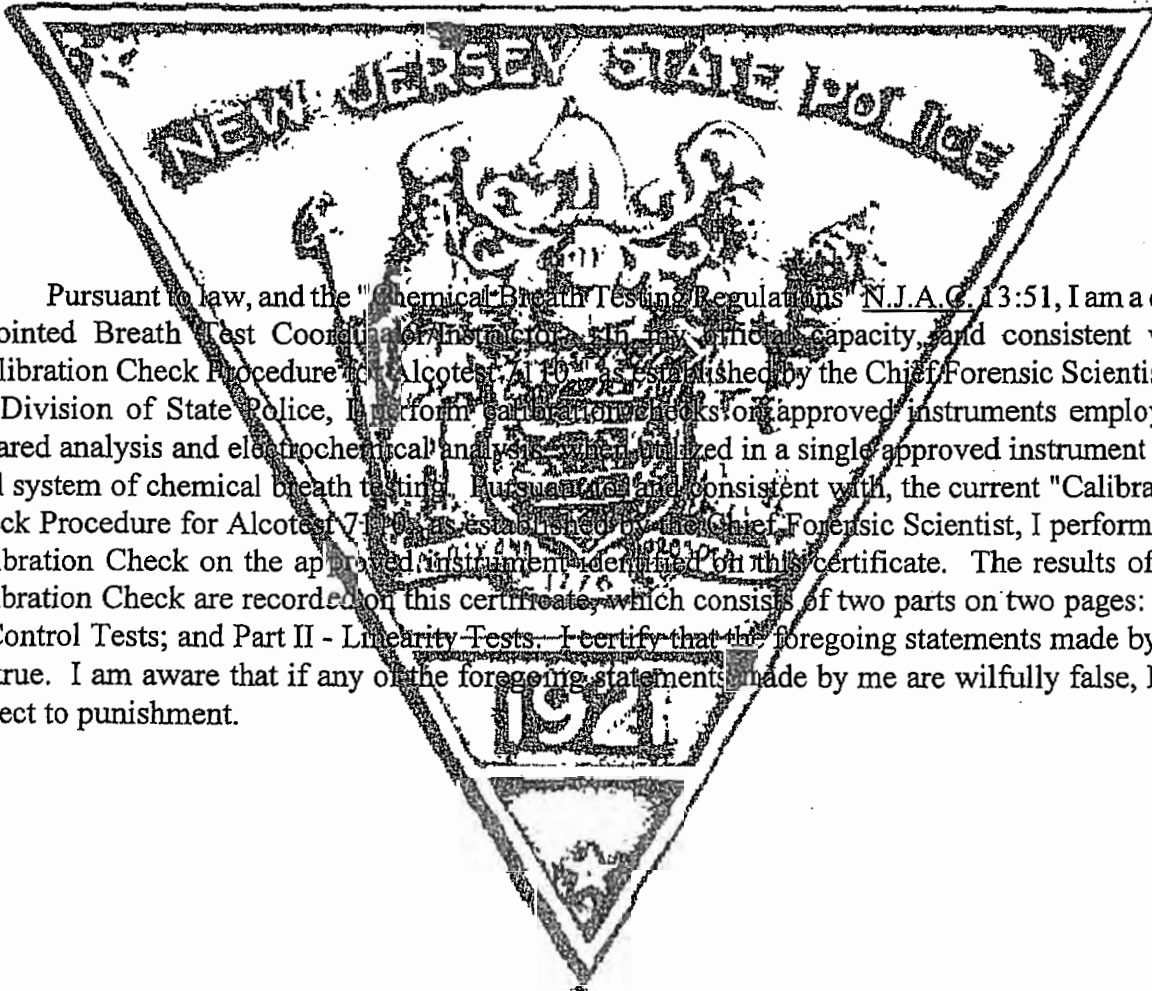

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
**Location:** LONGPORT POLICE  
**Calibration File No.:** 00256 **Calib. Date:** 08/26/2008 **Calib. No.:** 00005  
**Certification File No.:** 00257 **Cert. Date:** 08/26/2008 **Cert. No.:** 00004  
**Linearity File No.:** 00213 **Lin. Date:** 03/28/2008 **Lin. No.:** 00003  
**Solution File No.:** 00247 **Soln. Date:** 08/15/2008 **Soln. No.:** 00052  
**Sequential File No.:** 00257 **File Date:** 08/26/2008

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDXC S3-0154  
**Control Solution %:** 0.100% **Expires:** 02/22/2009  
**Solution Control Lot:** 07B045 **Bottle No.:** 0563

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:30D		
Control 1 EC	0.099%	09:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31D		
Control 2 EC	0.098%	09:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33D		
Control 3 EC	0.097%	09:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		

All tests within acceptable tolerances.

**Coordinator**  
Last Name: DEL ANOCE First Name: JOSEPH MI: S  
Signature: *J. Del Anoce # 6027* Badge No: 6027 Date: 08/26/2008

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor, in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0067  
Location: LONGPORT POLICE  
Calibration File No.: 00256 Calib. Date: 08/26/2008 Calib. No.: 00005  
Certification File No.: 00257 Cert. Date: 08/26/2008 Cert. No.: 00004  
Linearity File No.: 00258 Lin. Date: 08/26/2008 Lin. No.: 00004  
Solution File No.: 00247 Soln. Date: 08/15/2008 Soln. No.: 00052  
Sequential File No.: 00258 File Date: 08/26/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0196  
Control Solution %: 0.040% Expires: 01/26/2009  
Solution Control Lot: 07A041 Bottle No.: 0542

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0203  
Control Solution %: 0.080% Expires: 01/26/2009  
Solution Control Lot: 07A042 Bottle No.: 0308

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0205  
Control Solution %: 0.160% Expires: 01/26/2009  
Solution Control Lot: 07A043 Bottle No.: 0053

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:50D		
Control 1 EC	0.040%	09:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.038%	09:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52D		
Control 2 EC	0.040%	09:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		
Control 3 EC	0.079%	09:54D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.078%	09:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56D		
Control 4 EC	0.079%	09:56D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58D		
Control 5 EC	0.157%	09:58D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.156%	09:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00D		
Control 6 EC	0.156%	10:01D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.157%	10:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02D		

All tests within acceptable tolerance.

### Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: \_\_\_\_\_

*J. Dellanoce* #6027

Badge No.: 6027

Date: 08/26/2008

DEPARTMENT OF

Motor and Public Safety

This is to certify that

Joseph S. Ballanocce

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT PHYSICAL FITNESS ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1948 IN THE OPERATION OF THE Breathalyzer  
A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 13th DAY OF Dec.  
TWO THOUSAND AND 01

*Ken P. ...*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*...*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 8/30 - 9/3/99

Refresher Course

1.	DATE	PEACE	INSTRUCTOR
	12/12/01	A.G.P.C.	Porter
2.	2-2-03	CEPA	C. P. ...
3.	10-3-05	ACTE	A. ...
4.			
5.			
6.			
7.			
8.			
9.			

SP-293B (Rev. 4/00)



DEPARTMENT OF  
*Law and Public Safety*  
 This is to certify that

Joseph S. Dellanoce  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL-BREATH ANALYSES PURSUANT TO CHAPTER 12 OF  
 THE LAWS OF 1964 IN THE OPERATION OF THE Alcotest 7110 MKII-C  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND

Five

DAY OF March

*Joseph S. Dellanoce*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*Joseph S. Dellanoce*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	2-15-07	GCPA	C. POTER
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 293B (Rev. 12/04)

**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-016

Certification date:

04.04.08

Next Certification due:

04.04.09

Probe Value

106

Draeger Safety Diagnostics, Inc.  
Technical Service Department





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 WEST TRENTON NJ 08628-0668  
 (609) 882-2000

STUART RABNER  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

RON CORZINE  
 Governor

**CERTIFICATION OF ANALYSIS**  
**0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A041

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Ajit R. Tungare*

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

*Linda L. DeSantis*  
 Notary

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2008



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

STUART RABNER  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

RON CORZINE  
 Governor

**CERTIFICATION OF ANALYSIS**  
**0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A042

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0965 to 0.0972 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Ajit R. Tungare*

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

*Linda L. DeSantis*  
 Notary

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

RON S. CORZINE  
 Governor

STUART RABNER  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 04/04/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B045

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 22, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 20<sup>th</sup> day of April, 2007.

Notary

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

STUART RABNER  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

ION S. CORZINE  
 Governor

**CERTIFICATION OF ANALYSIS**  
**0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A043

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1932 to 0.1938 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2008

*Ajit R. Tungare*  
 Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

*Linda L. DeSantis*  
 Notary



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





Draeger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST<sup>®</sup> CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWE 53-0196

Certification Date

Technician

Re-Certification Due Date

02-13-08

VE

02-13-09



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWES3-0203

Certification Date

Technician


Re-Certification Due Date

02-13-08

*[Signature]*

02-13-09





Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST<sup>®</sup> CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

02-13-08

AL

02-13-09

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00256	Calib. Date: 08/26/2008
Certification File No.:	00257	Calib. No.: 00005
Linearity File No.:	00258	Cert. Date: 08/26/2008
Solution File No.:	00259	Cert. No.: 00004
Sequential File No.:	00259	Lin. Date: 08/26/2008
		Lin. No.: 00004
		Soln. Date: 08/26/2008
		Soln. No.: 00053
		File Date: 08/26/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 0510

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:09D		
Control 1 EC	0.101%	11:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10D		
Control 2 EC	0.099%	11:10D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:11D		
Control 3 EC	0.099%	11:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*TEMPERATURE PROBE SERIAL NUMBER: DDWAP2 - 177<sup>QSD</sup>*

**Changed By:**

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: \_\_\_\_\_

*J.P. Dellanoce # 6027*

Badge No.: 6027

Date: 08/26/2008



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE Box 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 03/14/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08B050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1229 to 0.1234 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 13, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Ajit R. Tungare*

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 31<sup>st</sup> day of March, 2008.

*Linda L. DeSantis*

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable

