

ALCOTEST CHECKLIST

Municipality: LONGPORT

Alcotest Ser. #: ARXA-0067

County: ATLANTIC

Date of Calibration: 09-29-2022

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC 53-0135

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWA P2-199

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 210 216 827

5. **NIST - Traceable Digital Thermometer Readings.**

6. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDEE P2-060

7. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

| | | |
|--|-----------------|--------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution. | <u>21250</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution. | <u>21260</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution. | <u>21210</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution. | <u>21290</u> |

8. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing. DDWE 53-0211
 B. 0.08% used in Calibration/Linearity Testing. DDXC 53-0020
 C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 D. 0.16% used in Calibration/Linearity Testing. DDMK 53-0008

9. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 21270
 D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest® 7110 MKII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

1-10-14

SERIAL NUMBER:

ARXA-00007

Dräger Safety Diagnostics, Inc.

BC

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDXCS3-0135

Certification Date:

4.29.22

Technician:

MB

Re-Certification Due Date:

4.29.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDWAP2-199

Certification Date:

4.29.22

Next Certification Due:

4.29.23

Probe Value:

104

Draeger, Inc.

MB



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064543

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 210216827 Manufacturer: Control Company

Standards/Equipment:

| Description | Serial Number | Due Date | NIST Traceable Reference |
|------------------------------|---------------|-------------|--------------------------|
| Thermistor Module | A27129 | 01 Mar 2022 | 1000464856 |
| Temperature Calibration Bath | A45240 | | |
| Temperature Calibration Bath | A73332 | | |
| Temperature Calibration Bath | B01976 | | |
| Temperature Probe | 5394 | 08 Mar 2022 | C1228019 |
| Temperature Calibration Bath | B3A444 | | |
| Temperature Probe | 5357 | 09 Jun 2021 | C0428083 |
| Thermistor Module | B5C344 | 06 Jun 2021 | 1000452872 |
| Thermistor Module | B98381 | 21 Aug 2021 | 1000457544 |
| Temperature Probe | 5392 | 04 Aug 2021 | C0804052 |
| Temperature Probe | 5398 | 04 Aug 2021 | C0804051 |

Certificate Information:

Technician: 420 Procedure: CAL-06 Cal Date: 17 Mar 2021 Cal Due Date: 17 Mar 2023
Test Conditions: 62.18%RH 22.28°C 1006mBar

Calibration Data: (New Instrument)

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min | Max | ±U | TUR |
|---------|---------|----------|--------|---------|---------|--------|--------|--------|--------|------|
| °C | N.A. | N.A. | | 0.000 | 0.000 | Y | -0.05 | 0.05 | 0.0087 | >4:1 |
| °C | N.A. | N.A. | | 24.000 | 24.002 | Y | 24.849 | 25.049 | 0.0087 | >4:1 |
| °C | N.A. | N.A. | | 50.001 | 50.001 | Y | 49.951 | 50.051 | 0.0087 | >4:1 |
| °C | N.A. | N.A. | | 100.000 | 99.999 | Y | 99.95 | 100.05 | 0.0087 | >4:1 |

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement (GUM). This uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ± U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Marisa Elms
Marisa Elms, Technical Manager

Note

Maintaining Accuracy:

In our opinion, once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77698
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CEIT-01009-2008-A0-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-12064543

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date 17 Mar 2021

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.tracoabfo.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB,
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr I Dennis J Lutz
Name

7045
Badge No.

Location:

Longport Police
Agency

ARXA-0067
Alcotest Serial No.

Equipment:

210 216 827
Digital NIST Temperature Measuring System Serial No.

| Simulator Solution Concentration | CU-34 Simulator Serial No. | Time Simulators Started to Heat | Time Temp. Reading Obtained | Temp. Reading on NIST Traceable Thermometer |
|----------------------------------|----------------------------|---------------------------------|-----------------------------|---|
| 0.04% | DDWE S3-0211 | 07:45 D | 08:47 D | 33.9°C |
| 0.08% | DDXC S3-0020 | 07:45 D | 08:48 D | 33.9°C |
| 0.10% | DDXC S3-0135 | 07:45 D | 08:50 D | 33.8°C |
| 0.16% | DDMK S3-0008 | 07:45 D | 08:51 D | 34.0°C |

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius ± 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I Lutz 7045
Coordinator's Signature

9-29-22
Date

Alcotest 7110 Calibration Record

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00970 Calib. Date: 09/29/2022 Calib. No.: 00042
Certification File No.: 00956 Cert. Date: 05/05/2022 Cert. No.: 00035
Linearity File No.: 00957 Lin. Date: 05/05/2022 Lin. No.: 00035
Solution File No.: 00967 Soln. Date: 09/06/2022 Soln. No.: 00269
Sequential File No.: 00970 File Date: 09/29/2022


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 06/16/2023
Solution Control Lot: 21210 Bottle No.: 1118

Coordinator

Last Name: LUTZ First Name: DENNIS MI: J
Signature: Tpr I Dent 7045 Badge No.: 7045
Date: 09/29/2022

*Black Key Temperature Probe Serial.....# DDEE P2-060 (DL)
*Digital NIST Temperature Measuring System Serial.....# 210 216 827 (DL)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police; I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

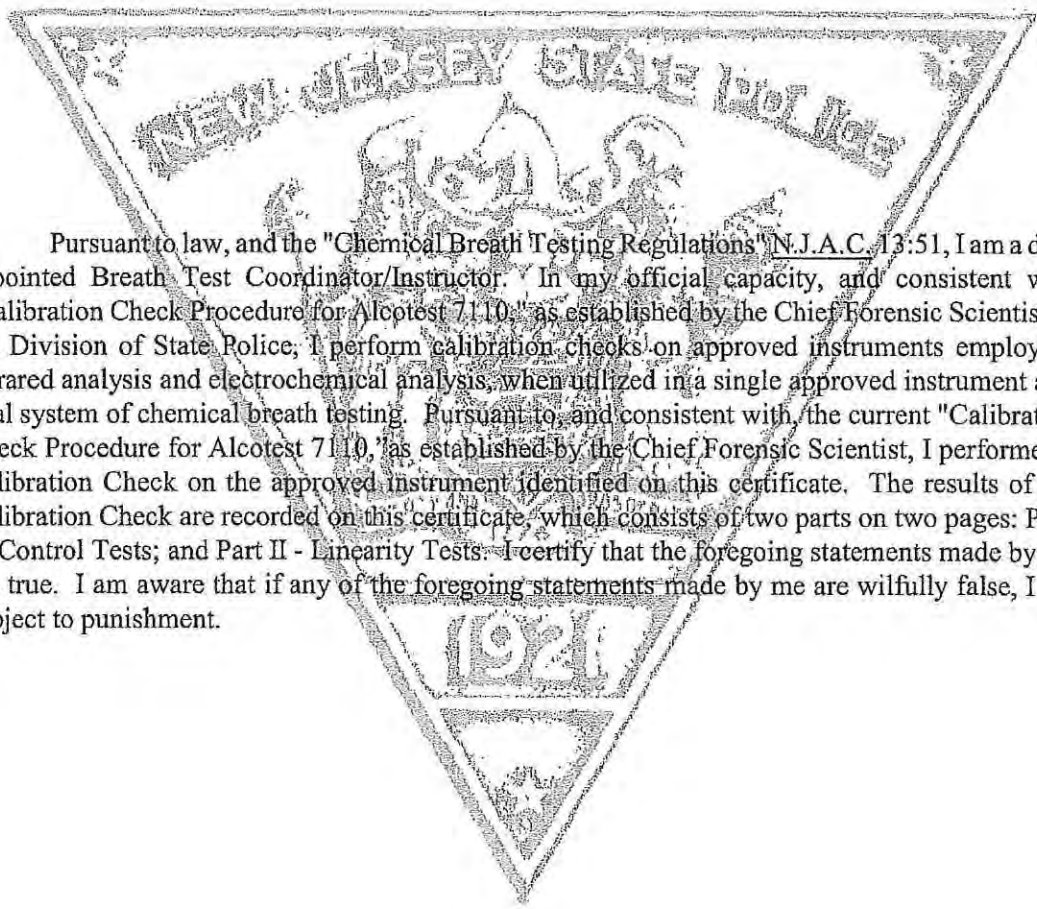

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00970 Calib. Date: 09/29/2022 Calib. No.: 00042
Certification File No.: 00971 Cert. Date: 09/29/2022 Cert. No.: 00036
Linearity File No.: 00957 Lin. Date: 05/05/2022 Lin. No.: 00035
Solution File No.: 00967 Soln. Date: 09/06/2022 Soln. No.: 00269
Sequential File No.: 00971 File Date: 09/29/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 06/16/2023
Solution Control Lot: 21210 Bottle No.: 1118

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 09:03D | | |
| Control 1 EC | 0.100% | 09:03D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 09:03D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:04D | | |
| Control 2 EC | 0.098% | 09:05D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 09:05D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:05D | | |
| Control 3 EC | 0.099% | 09:06D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 09:06D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:07D | | |

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpr I [Signature]

Badge No.: 7045

Date: 09/29/2022

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00970 Calib. Date: 09/29/2022 Calib. No.: 00042
Certification File No.: 00971 Cert. Date: 09/29/2022 Cert. No.: 00036
Linearity File No.: 00972 Lin. Date: 09/29/2022 Lin. No.: 00036
Solution File No.: 00967 Soln. Date: 09/06/2022 Soln. No.: 00269
Sequential File No.: 00972 File Date: 09/29/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0211
Control Solution %: 0.040% Expires: 07/06/2023
Solution Control Lot: 21250 Bottle No.: 0275

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0020
Control Solution %: 0.080% Expires: 07/19/2023
Solution Control Lot: 21260 Bottle No.: 1358

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0008
Control Solution %: 0.160% Expires: 07/29/2023
Solution Control Lot: 21290 Bottle No.: 1432

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 09:23D | | |
| Control 1 EC | 0.041% | 09:24D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.041% | 09:24D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:25D | | |
| Control 2 EC | 0.041% | 09:26D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.040% | 09:26D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:27D | | |
| Control 3 EC | 0.081% | 09:28D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.082% | 09:28D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:30D | | |
| Control 4 EC | 0.081% | 09:31D | 34.0°C | *** TEST PASSED *** |
| Control 4 IR | 0.081% | 09:31D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:32D | | |
| Control 5 EC | 0.162% | 09:33D | 34.0°C | *** TEST PASSED *** |
| Control 5 IR | 0.163% | 09:33D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:34D | | |
| Control 6 EC | 0.161% | 09:35D | 34.0°C | *** TEST PASSED *** |
| Control 6 IR | 0.162% | 09:35D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:37D | | |

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS


MI: J

Signature: _____

Tpr I Dennis 7045

Badge No.: 7045

Date: 09/29/2022



Dennis J. Lutz

Breath Test Coordinator/Instructor

REGISTRATION AND CERTIFICATION TO OPERATE COMPACT BREATHALYZERS AND INSTRUMENTS TO OPERATE UNDER

THE RULES OF THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

APPROVED BY THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

EXPIRES ON 12/31/13 AT 11:59 PM

ISSUED AT MOBILE BY [Signature]

STATE OF ALABAMA DEPARTMENT OF PUBLIC SAFETY

ORIGINAL COURSE DATES

| DATE | Full/Short Course PLACE | INSTRUCTOR |
|------|-------------------------|------------|
| 1. | | |
| 2. | | |
| 3. | | |
| 4. | | |
| 5. | | |
| 6. | | |
| 7. | | |
| 8. | | |
| 9. | | |
| 10. | | |

ORIGINAL COURSE DATES

| DATE | Full/Short Course PLACE | INSTRUCTOR |
|-------------|-------------------------|-----------------|
| 1. 2-3-11 | OCFA | W. H. H. |
| 2. 1/24/13 | OCFA | Chris Stead |
| 3. 11-23-13 | CCPA | N. Gonzalez |
| 4. 4/6/17 | LAKEMONT | Adam Stead |
| 5. 9/22/19 | NEP Galloway | R. [Signature] |
| 6. 7-19-21 | Lakemont | Jim [Signature] |
| 7. | | |
| 8. | | |
| 9. | | |
| 10. | | |



New Jersey State Police

IN COMPLIANCE AND CONFORMANCE WITH THE RULES OF THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

APPROVED BY THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

EXPIRES ON 10/31/13 AT 11:59 PM

ISSUED AT MOBILE BY [Signature]

STATE OF ALABAMA DEPARTMENT OF PUBLIC SAFETY

REGISTRATION AND CERTIFICATION TO OPERATE COMPACT BREATHALYZERS AND INSTRUMENTS TO OPERATE UNDER

THE RULES OF THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

APPROVED BY THE BOARD OF PUBLIC SAFETY, ALABAMA TITLE 330

EXPIRES ON 10/31/13 AT 11:59 PM

ISSUED AT MOBILE BY [Signature]

STATE OF ALABAMA DEPARTMENT OF PUBLIC SAFETY



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

PHILIP D. MURPHY
 Governor

SHEILA Y. OLIVER
 Lt. Governor

GURHIR S. GREWAL
 Attorney General

PATRICK J. CALLAHAN
 Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
 Michael Kennedy
 Assistant Chief Forensic Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.
Karen E. Stahl
 Notary

KAREN E. STAHL
 NOTARY PUBLIC OF NEW JERSEY
 Commission # 50110822
 My Commission Expires 8/19/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRANTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0970 to 0.0977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 00110522
My Commission Expires 6/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 07/07/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1199 to 0.1215 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 16, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy

Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 08 day of July, 2021.
Karen E. Stahl
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2600

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/11/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1945 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 29, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Karen E. Stahl
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 80110522
My Commission Expires 07/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDWES3-0211

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDXCS3-0020

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDMK53-0008

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-060

Certification Date:

4.1.22

Next Certification Due:

4.1.23

Probe Value:

104

Dräger, Inc.

MB

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARXA-0067 |
| Location: | LONGPORT POLICE | |
| Calibration File No.: | 00970 | Calib. Date: 09/29/2022 |
| Certification File No.: | 00971 | Calib. No.: 00042 |
| Linearity File No.: | 00972 | Cert. Date: 09/29/2022 |
| Solution File No.: | 00973 | Cert. No.: 00036 |
| Sequential File No.: | 00973 | Lin. Date: 09/29/2022 |
| | | Lin. No.: 00036 |
| | | Soln. Date: 09/29/2022 |
| | | Soln. No.: 00270 |
| | | File Date: 09/29/2022 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDXC S3-0135 |
| Solution Control Lot: | 21270 | Expires: 07/21/2023 |
| | | Bottle No.: 0280 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 10:48D | | |
| Control 1 EC | 0.100% | 10:49D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 10:49D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:49D | | |
| Control 2 EC | 0.099% | 10:50D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 10:50D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:51D | | |
| Control 3 EC | 0.098% | 10:51D | 33.9°C | *** TEST PASSED *** |
| Control 3 IR | 0.101% | 10:51D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:52D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-199 DL

Changed By:

Last Name: LUTZ First Name: DENNIS MI: J

Signature: Tpc I [Signature] 7045 Badge No.: 7045

Date: 09/29/2022



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/10/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1208 to 0.1221 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 21, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 01/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

