

ALCOTEST CHECKLIST

Municipality: LONGPORT Alcotest Ser. #: ARXA-0067

County: ATLANTIC Date of Calibration: 10-20-2017

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.

2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXC S3-0135

3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DOWA P2-199

4. **Digital Temperature Measuring System Report of Calibration.**
Ser. #: 170 428 368

5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDXK P2-396

6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:

<input checked="" type="checkbox"/> A.	0.04% Solution.	<u>16230</u>
<input checked="" type="checkbox"/> B.	0.08% Solution.	<u>16250</u>
<input checked="" type="checkbox"/> C.	0.10% Solution.	<u>16220</u>
<input checked="" type="checkbox"/> D.	0.16% Solution.	<u>16260</u>

7. **Certificate of Accuracy Alcotest CU34 Simulators** from Draeger Safety (when conducting the Calibration/Linearity Tests) for:

A. 0.04% used in Calibration/Linearity Testing. DDWE S3-0206
 B. 0.08% used in Calibration/Linearity Testing. DDWF S3-0218
 C. 0.10% used in Calibration/Linearity Testing.
[Same as CU34 unit on instrument.]
 D. 0.16% used in Calibration/Linearity Testing. DDWJ S3-0334

8. A. New Standard Solution Report following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 17050
 D. Alcotest card of operator/coordinator who completed change.

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


1-10-14

SERIAL NUMBER:

ARXA-00107

Dräger Safety Diagnostics, Inc.

BC



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXCS3-0135

Certification Date

6-6-17

Technician

72

Re-Certification Due Date

6-6-18

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-199

Certification date:

6-12-17

Next Certification due:

6-12-18

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department

72



Calibration
Certificate No. 1750.01

**Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001**



Cert. No.: 4000-8609168

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087
Instrument Identification:

Model: 61220-601 S/N: 170428368 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/17 Due Date: 6/08/19
Test Conditions: 23.5°C 50.0 %RH 1014 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	0.001	Y	-0.048	0.052	0.010	>4.1
°C		N.A.		25.003	25.000	Y	24.953	25.053	0.010	>4.1
°C		N.A.		50.002	50.001	Y	49.952	50.052	0.010	>4.1
°C		N.A.		100.001	99.998	Y	99.951	100.051	0.010	>4.1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Justice
Aaron Justice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: LONGPORT POLICE
Calibration File No.: 00827
Certification File No.: 00816
Linearity File No.: 00817
Solution File No.: 00826
Sequential File No.: 00827

Calib. Date: 10/20/2017
Cert. Date: 06/05/2017
Lin. Date: 06/05/2017
Soln. Date: 09/14/2017
File Date: 10/20/2017

Serial No.: ARXA-0067
Calib. No.: 00031
Cert. No.: 00024
Lin. No.: 00024
Soln. No.: 00204

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 16220

Model No.: CU-34

Serial No.: DDXC S3-0135
Expires: 09/07/2018
Bottle No.: 0619

Coordinator

Last Name: ALCOTT

First Name: KEVIN


MI: W.

Signature: Tpr. I K W. Q #6704

Badge No.: 6704

Date: 10/20/2017

*Black Key Temperature Probe Serial.....# DDXKP2-396 (KA)
*Digital NIST Temperature Measuring System Serial.....# 170 428 368 (KA)

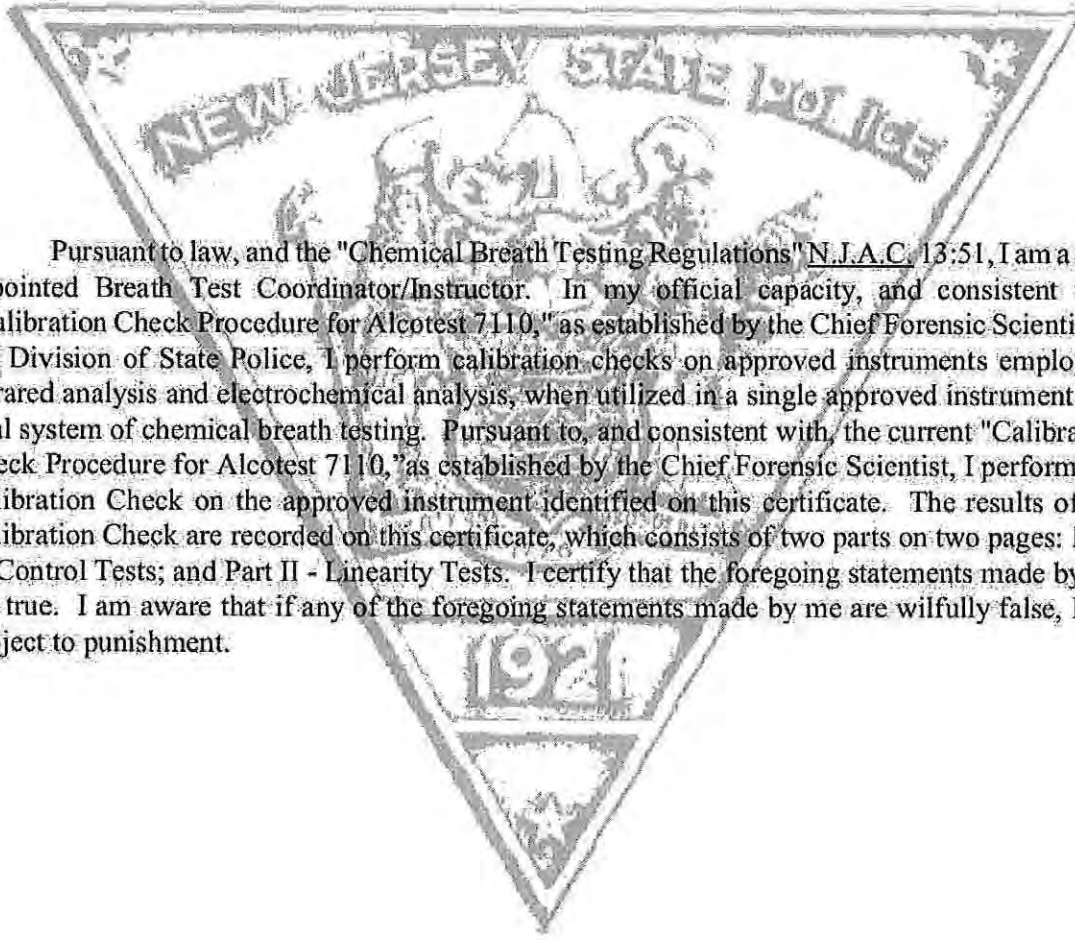

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00827 Calib. Date: 10/20/2017 Calib. No.: 00031
Certification File No.: 00828 Cert. Date: 10/20/2017 Cert. No.: 00025
Linearity File No.: 00817 Lin. Date: 06/05/2017 Lin. No.: 00024
Solution File No.: 00826 Soln. Date: 09/14/2017 Soln. No.: 00204
Sequential File No.: 00828 File Date: 10/20/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 09/07/2018
Solution Control Lot: 16220 Bottle No.: 0619

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:11D		
Control 1 EC	0.099%	13:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:12D		
Control 2 EC	0.098%	13:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14D		
Control 3 EC	0.098%	13:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:15D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Badge No.: 6704

Date: 10/20/2017

Signature: Tpr. I. K. W. #6704

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00827 Calib. Date: 10/20/2017 Calib. No.: 00031
Certification File No.: 00828 Cert. Date: 10/20/2017 Cert. No.: 00025
Linearity File No.: 00829 Lin. Date: 10/20/2017 Lin. No.: 00025
Solution File No.: 00826 Soln. Date: 09/14/2017 Soln. No.: 00204
Sequential File No.: 00829 File Date: 10/20/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0206
Control Solution %: 0.040% Expires: 09/19/2018
Solution Control Lot: 16230 Bottle No.: 0642

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0218
Control Solution %: 0.080% Expires: 09/27/2018
Solution Control Lot: 16250 Bottle No.: 1437

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0334
Control Solution %: 0.160% Expires: 10/03/2018
Solution Control Lot: 16260 Bottle No.: 0284

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:30D		
Control 1 EC	0.042%	13:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	13:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:32D		
Control 2 EC	0.040%	13:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	13:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:34D		
Control 3 EC	0.080%	13:35D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	13:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:36D		
Control 4 EC	0.080%	13:37D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	13:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39D		
Control 5 EC	0.159%	13:40D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	13:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41D		
Control 6 EC	0.159%	13:42D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	13:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:44D		

All tests within acceptable tolerance.

Coordinator

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: Tpr. I K W. #6704

Badge No.: 6704

Date: 10/20/2017

DEPARTMENT OF
Traffic and Public Safety
Whose is to certify that

Kevin W. Alcott

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 21st DAY OF May TWO THOUSAND AND Fifteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2028 (Rev. 08/13)

DEPARTMENT OF
Traffic and Public Safety
Whose is to certify that

KEVIN W. ALCOTT

NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 21st DAY OF APRIL TWO THOUSAND AND EIGHT

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 8-25-10	BCPA	R. Tan
2. 1-12-12	Berlin WPA	C. Tan
3. 1-16-14	SAYREVILLE PD	R. Tan
4. 1/21/16	Lakewood	Adam Standa
5.		
6.		
7.		
8.		
9.		

S.P. 2028 (Rev. 07/07)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/27/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0492 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 19, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaoui, Ph.D.,
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of September, 2016.

[Signature]
Notary
MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. PUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/04/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0965 to 0.0975 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 27, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 5th day of October, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"
New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CURIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. PUNTERO
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/19/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1207 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 07, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19th day of September, 2016.

[Signature]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/13/2016

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 16260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1928 to 0.1964 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 17 day of October, 2016.

Notary
JOHN R LEAVER
ID # 2207138
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer.
Printed on Recycled Paper and Recyclable



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWES3-0206

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWFS3-0218

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDWJ53-0334

Certification Date:

9-27-17

Technician:

BC

Re-Certification Due Date:

9-27-18

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-396

Certification Date:

9-8-17

Next Certification Due:

9-8-18

Probe Value:

104

Draeger, Inc.

BC

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00827 Calib. Date: 10/20/2017 Calib. No.: 00031
Certification File No.: 00828 Cert. Date: 10/20/2017 Cert. No.: 00025
Linearity File No.: 00829 Lin. Date: 10/20/2017 Lin. No.: 00025
Solution File No.: 00830 Soln. Date: 10/20/2017 Soln. No.: 00205
Sequential File No.: 00830 File Date: 10/20/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/30/2019
Solution Control Lot: 17050 Bottle No.: 1120

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:53D		
Control 1 EC	0.099%	14:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54D		
Control 2 EC	0.099%	14:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:56D		
Control 3 EC	0.098%	14:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: ΔΔWAPZ-199 (KA)

Changed By:

Last Name: ALCOTT

First Name: KEVIN

MI: W.

Signature: TPT. I K W. #6704

Badge No.: 6704

Date: 10/20/2017



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor
KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 02/13/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1213 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 30, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaoui]

Ali M. Alaoui, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 16th day of February, 2017.

[Handwritten signature of Mary Elizabeth McLaughlin]
Notary

MARY ELIZABETH MCLAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

