

ALCOTEST CHECKLIST

Municipality: BUENA BORO

Alcotest Ser.#: ARXB-0074

County: ATLANTIC

Date of Calibration: 10-05-2009

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.
Ser. #: DDXJ S3-0210
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.
Ser. #: DDWT P2-204
4. **Digital Temperature Measuring System Report of Calibration.**
5. A. Alcotest 7110 Calibration Record
 B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
 C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
 D. **Alcotest Card** of operator/coordinator who performed tests.
 E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].
Ser. #: DDWA P2-016
6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
- | | | | | |
|--|-----------------|-----------|----------|------------|
| <input checked="" type="checkbox"/> A. | 0.04% Solution. | <u>08</u> | <u>F</u> | <u>054</u> |
| <input checked="" type="checkbox"/> B. | 0.08% Solution. | <u>08</u> | <u>F</u> | <u>055</u> |
| <input checked="" type="checkbox"/> C. | 0.10% Solution. | <u>08</u> | <u>G</u> | <u>056</u> |
| <input checked="" type="checkbox"/> D. | 0.16% Solution. | <u>08</u> | <u>G</u> | <u>057</u> |
7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
- A. 0.04% used in Calibration/Linearity Testing DDWE S3-0196
- B. 0.08% used in Calibration/Linearity Testing DDWE S3-0203
- C. 0.10% used in Calibration/Linearity Testing DDXJ S3-0210
[Same as instrument's CU34 unit].
- D. 0.16% used in Calibration/Linearity Testing DDWE S3-0205
8. A. New Standard Solution Report - following Calibration.
 B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
 C. Certificate of Analysis 0.10% solution for same.
Lot #: 08 B 050
 D. Alcotest card of operator/coordinator who completed change.

TJP

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

08/04/2000

SERIAL NUMBER:

ARXB-0074

Draeger Safety Diagnostics, Inc.
Durango, CO

Carl Dly



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

20X552-0210

Certification Date

Technician

Re-Certification Due Date

10-08-2008

JS

10-08-2009

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

22WJPR-204

Certification date:

10-08-2008

Next Certification due:

10-08-2009

Probe Value

104

Dräger Safety Diagnostics, Inc.
Technical Service Department

JS



Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NCSL Z540-1



Cert. No.: 4000-2035927

Traceable® Certificate of Calibration for Digital Thermometer

Instrument Identification:

Model: 61220-601 S/N: 80637585 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Probe	149	3/08/09	A82225037-3
Thermistor Module	A27129	8/22/09	1000248949
Temperature Calibration Bath TC218	A73332		
Temperature Calibration Bath TC155	83139		
Thermistor Module	A27129	8/22/09	1000248949
Temperature Probe	157	5/28/09	A8519038-4

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 11/18/08 Cal Due: 11/18/10
Test Conditions: 25.0°C 34.0 %RH 1031 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±uc	TUR
°C		N.A.		0.001	-0.002	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.001	25.003	Y	24.951	25.051	0.013	3.8:1
°C		N.A.		60.001	59.998	Y	59.951	60.051	0.018	2.8:1
°C		N.A.		100.001	100.001	Y	99.951	100.051	0.013	3.8:1

This instrument was calibrated using instruments Traceable to National Institute of Standards and Technology. :

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Date=MM/DD/YYYY

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77548 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-AQ-HOU.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Alcotest 7110 Calibration Record


Equipment Alcotest 7110 MKIII-C Serial No.: ARXB-0074
Location: BUENA BOROUGH POLICE
Calibration File No.: 00039 Calib. Date: 10/05/2009 Calib. No.: 00004
Certification File No.: 00023 Cert. Date: 04/24/2009 Cert. No.: 00002
Linearity File No.: 00024 Lin. Date: 04/24/2009 Lin. No.: 00002
Solution File No.: 00037 Soln. Date: 09/03/2009 Soln. No.: 00016
Sequential File No.: 00039 File Date: 10/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXJ S3-0210
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 0535

Coordinator

Last Name: DELLANOCE First Name: JOSEPH MI: S
Signature: Tpr. II J. Dellanoce # 6027 Badge No.: 6027
Date: 10/05/2009

*Black Key Temperature Probe Serial.....# DOWAP2-016 *jsd*
*Digital NIST Temperature Measuring System Serial.....# 80627585 *jsd*

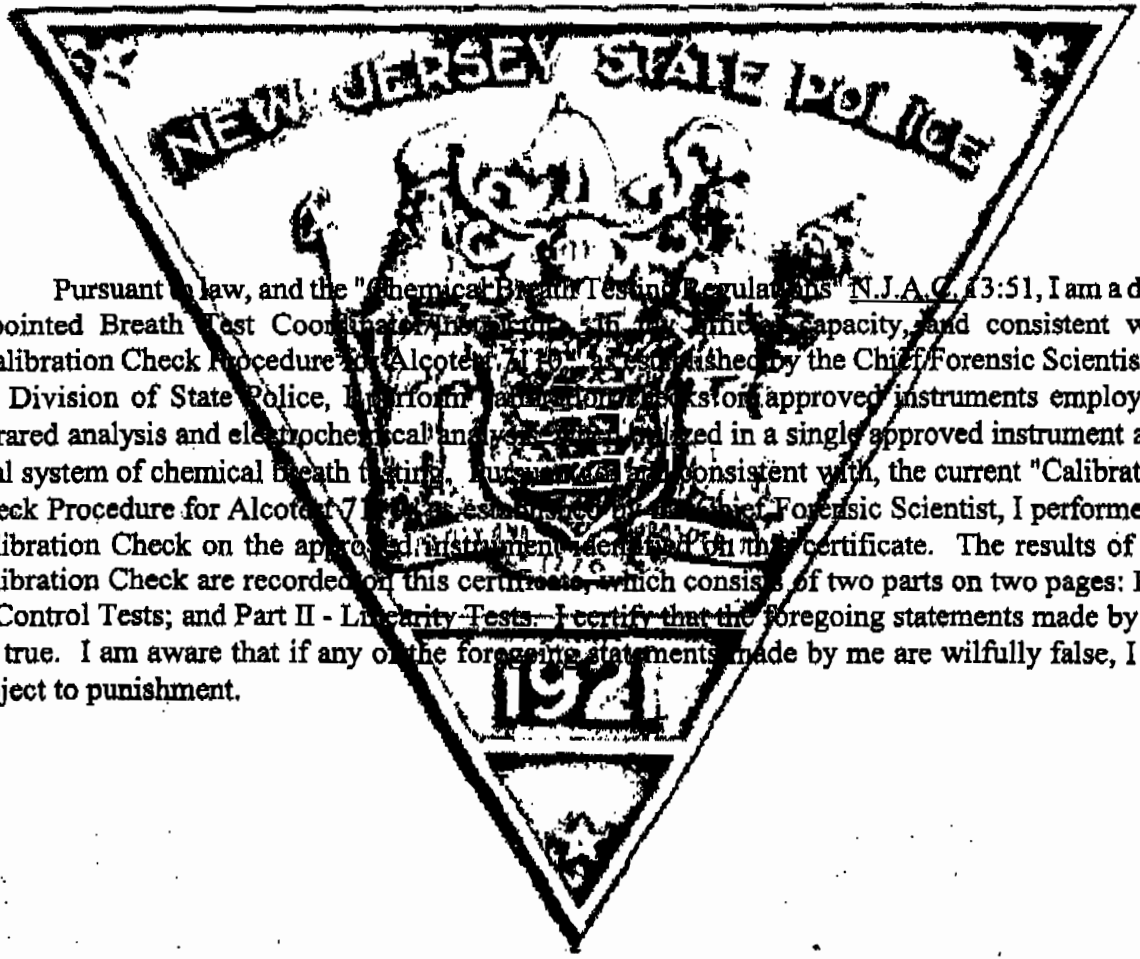

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, analyzed in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXB-0074
Location:	BUENA BOROUGH POLICE	
Calibration File No.:	00039	Calib. Date: 10/05/2009
Certification File No.:	00040	Calib. No.: 00004
Linearity File No.:	00024	Cert. Date: 10/05/2009
Solution File No.:	00037	Lin. Date: 04/24/2009
Sequential File No.:	00040	Soln. Date: 09/03/2009
		Soln. No.: 00016
		File Date: 10/05/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXJ S3-0210
Solution Control Lot:	08G056	Expires: 07/02/2010
		Bottle No.: 0535

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:46D		
Control 1 EC	0.100%	11:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48D		
Control 2 EC	0.098%	11:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:49D		
Control 3 EC	0.098%	11:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50D		

All tests within acceptable tolerance.

Coordinator: **Last Name:** DELANOCE **First Name:** JOSEPH **Badge No.:** 6027 **Date:** 10/05/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, which are realized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Alcotest 7110 MKIII-C
Location: BUENA BOROUGH POLICE
Serial No.: ARXB-0074
Calibration File No.: 00039
Cert. Date: 10/05/2009
Calib. No.: 00004
Certification File No.: 00040
Cert. Date: 10/05/2009
Cert. No.: 00003
Linearity File No.: 00041
Lin. Date: 10/05/2009
Lin. No.: 00003
Solution File No.: 00037
Soln. Date: 09/03/2009
Soln. No.: 00016
Sequential File No.: 00041
File Date: 10/05/2009

Calibrating Unit: WET
Control Solution %: 0.040%
Solution Control Lot: 08F054
Model No.: CU-34
Serial No.: DDWE S3-0196
Expires: 06/26/2010
Bottle No.: 0458

Calibrating Unit: WET
Control Solution %: 0.080%
Solution Control Lot: 08F055
Model No.: CU-34
Serial No.: DDWE S3-0203
Expires: 06/28/2010
Bottle No.: 0958

Calibrating Unit: WET
Control Solution %: 0.160%
Solution Control Lot: 08G057
Model No.: CU-34
Serial No.: DDWE S3-0205
Expires: 07/07/2010
Bottle No.: 0814

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:05D		
Control 1 EC	0.041%	12:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	12:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07D		
Control 2 EC	0.040%	12:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	12:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:09D		
Control 3 EC	0.080%	12:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.078%	12:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:11D		
Control 4 EC	0.079%	12:12D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.078%	12:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:13D		
Control 5 EC	0.158%	12:14D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	12:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15D		
Control 6 EC	0.157%	12:16D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.158%	12:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:17D		

All tests within acceptable tolerance.

Coordinator

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Joseph Dellanoce # 6027

Badge No.: 6027

Date: 10/05/2009

DEPARTMENT OF
Police and Public Safety

This is to certify that
Joseph S. D'Alanoce
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT COURSE IN THE STATE POLICE TRAINING CENTER IN THE
 NAME OF THE DEPARTMENT OF POLICE AND PUBLIC SAFETY
 A METHOD TO DETERMINE QUALIFICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF March

TWO THOUSAND AND
[Signature]
 NEW JERSEY STATE POLICE

Five
[Signature]
 ATTENDING OFFICER
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2-15-87	CCPA	Porter
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 883B (Rev. 1-80)

DEPARTMENT OF
Fire and Public Safety

This is to certify that
Joseph B. Ballanocce
New Jersey State Police

is qualified and competent to use the **Respirator Analyzer**
in accordance with the provisions of the **Respirator**
and the **Method of Defeating Intoxicants**

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS
13th DAY OF Dec.
2001

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES: 6/90 - 9/3/99

	DATE	PLACE	INSTRUCTOR
1.	12/12/01	A.G.P.C.	NO. 1000
2.	2-20-03	ACPE	Ch. [Signature]
3.	10/3-09	ACPE	Ch. [Signature]
4.			
5.			
6.			
7.			
8.			
9.			

SP-293B (Rev. 4/00)

Dräger safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDN472-016

Certification date:

02/13/2009

Next Certification due:

02/03/2010

Probe Value

106

Dräger Safety Diagnostics, Inc.
Technical Service Department

[Signature]



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
West Trenton NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 07/16/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F054

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary
JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Draper Safety, Inc.

ANALYSIS DATE: 07/25/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 17th day of August, 2008.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TAUNTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/24/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G056

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1227 to 0.1236 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 2, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 13th day of August, 2008.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 01/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary

JOHN R. LEAVER
 NOTARY PUBLIC STATE OF NEW JERSEY
 MY COMMISSION EXPIRES 12/14/2012





Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 24 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0196

Certification Date

Technician

Re-Certification Due Date

02-03-09

[Signature]

02-03-10



Draeger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDW 53-0203

Certification Date

02-03-09

Technician

Re-Certification Due Date

02-03-10



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 248 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWES3-0205

Certification Date

Technician

Re-Certification Due Date

02-03-09

J.E.

02-03-10

Calibrating Unit New Standard Solution Report

Equipment

Location: BUENA BOROUGH POLICE
 Calibration File No.: 00039
 Certification File No.: 00040
 Linearity File No.: 00041
 Solution File No.: 00042
 Sequential File No.: 00042

Alcotest 7110 MKIII-C
 Calib. Date: 10/05/2009
 Cert. Date: 10/05/2009
 Lin. Date: 10/05/2009
 Soln. Date: 10/05/2009
 File Date: 10/05/2009

Serial No.: ARXB-0074
 Calib. No.: 00004
 Cert. No.: 00003
 Lin. No.: 00003
 Soln. No.: 00017

Calibrating Unit: WET
 Control Solution %: 0.100%
 Solution Control Lot: 08B050

Model No.: CU-34

Serial No.: DDXJ S3-0210
 Expires: 02/13/2010
 Bottle No.: 0493

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:24D		
Control 1 EC	0.100%	13:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	13:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:25D		
Control 2 EC	0.098%	13:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	13:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:26D		
Control 3 EC	0.098%	13:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWTP2-204_{gco}

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tr. II J. Dellanoce # 6027

Badge No.: 6027

Date: 10/05/2009



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 Post Office Box 7068
 WEST TAUNTON NJ 08628-0068
 (609) 882-2000

JEN S. CORZINE
 Governor

ANNE MILGRAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 03/14/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08B050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1229 to 0.1234 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 13, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
 Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 31 day of March, 2008.

Linda L. DeBantis

Linda L. DeBantis
 My Commission
 Expires Aug. 17, 2008



New Jersey is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

