

Municipality: BUENO BORO Alcotest Ser.#: ARXB-0074

ALCOTEST CHECKLIST

1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R..
2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDXJ S3-0209
3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R..  
Ser. #: DDWA P2-148
4. **Digital Temperature Measuring System Report of Calibration.**
5.
  - A. Alcotest 7110 Calibration Record
  - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
  - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
  - D. **Alcotest Card** of operator/coordinator who performed tests.
  - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDWA P2-024
6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
  - A. 0.04% Solution. 07A041
  - B. 0.08% Solution. 07A042
  - C. 0.10% Solution. 07B045
  - D. 0.16% Solution. 07A043
7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
  - A. 0.04% used in Calibration/Linearity Testing. DOWF S3-0221
  - B. 0.08% used in Calibration/Linearity Testing. DOWF S3-0223
  - C. 0.10% used in Calibration/Linearity Testing DDXJ S3-0209  
[Same as instrument's CU34 unit].
  - D. 0.16% used in Calibration/Linearity Testing. DDWF S3-0225
8.
  - A. New Standard Solution Report - following Calibration.
  - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
  - C. Certificate of Analysis 0.10% solution for same.  
Lot #: 08 B050
  - D. Alcotest card of operator/coordinator who completed change.

Dräger safety

Alcotest<sup>®</sup> 7110 MKIII-C

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705.

The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


08/04/2006

SERIAL NUMBER:

ARXB-0074

Draeger Safety Diagnostics, Inc.  
Durango, CO

Art Dly



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDXJS3-0209

Certification Date

04.04.08

Technician

[Signature]

Re-Certification Due Date

04.04.09

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAPZ-148

Certification date:

04.04.08

Next Certification due:

04.04.09

Probe Value

104

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

[Signature]

## Ertco-Hart Digital Temperature Measuring System

### REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature

verification Serial Number: HH4130316 / HH41303176 / MERCURY THERMOMETER


Digital Units Serial Number: A23730

Probe Serial Number: 773623

Certification Date: 02-13-08

Next Certification Due: 02-13-09

At 34.00 °C digital unit displays 34.07 °C

Draeger Safety Diagnostics, Inc. Technician: 

# Alcotest 7110 Calibration Record

**Equipment**

Alcotest 7110 MKIII-C  
Location: BUENA BOROUGH POLICE  
Serial No.: ARXB-0074

Calibration File No.:	00004	Calib. Date:	11/05/2008	Calib. No.:	00002
Certification File No.:	00000	Cert. Date:	--/------	Cert. No.:	00000
Linearity File No.:	00000	Lin. Date:	--/------	Lin. No.:	00000
Solution File No.:	00002	Soln. Date:	08/04/2006	Soln. No.:	00001
Sequential File No.:	00004	File Date:	11/05/2008		


Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXJ S3-0209
Control Solution %:	0.100%			Expires:	02/22/2009
Solution Control Lot:	07B045			Bottle No.:	0367

**Coordinator**

Last Name: STANKS  
First Name: ADAM  
MI: N  
Signature: TPR I Adam N Stanks #5403  
Badge No.: 5403  
Date: 11/05/2008

\*Black Key Temperature Probe Serial .....# DDWAP2-024 ans

\*Ertco-Hart Digital Temperature Measuring System Serial# A23730 ans

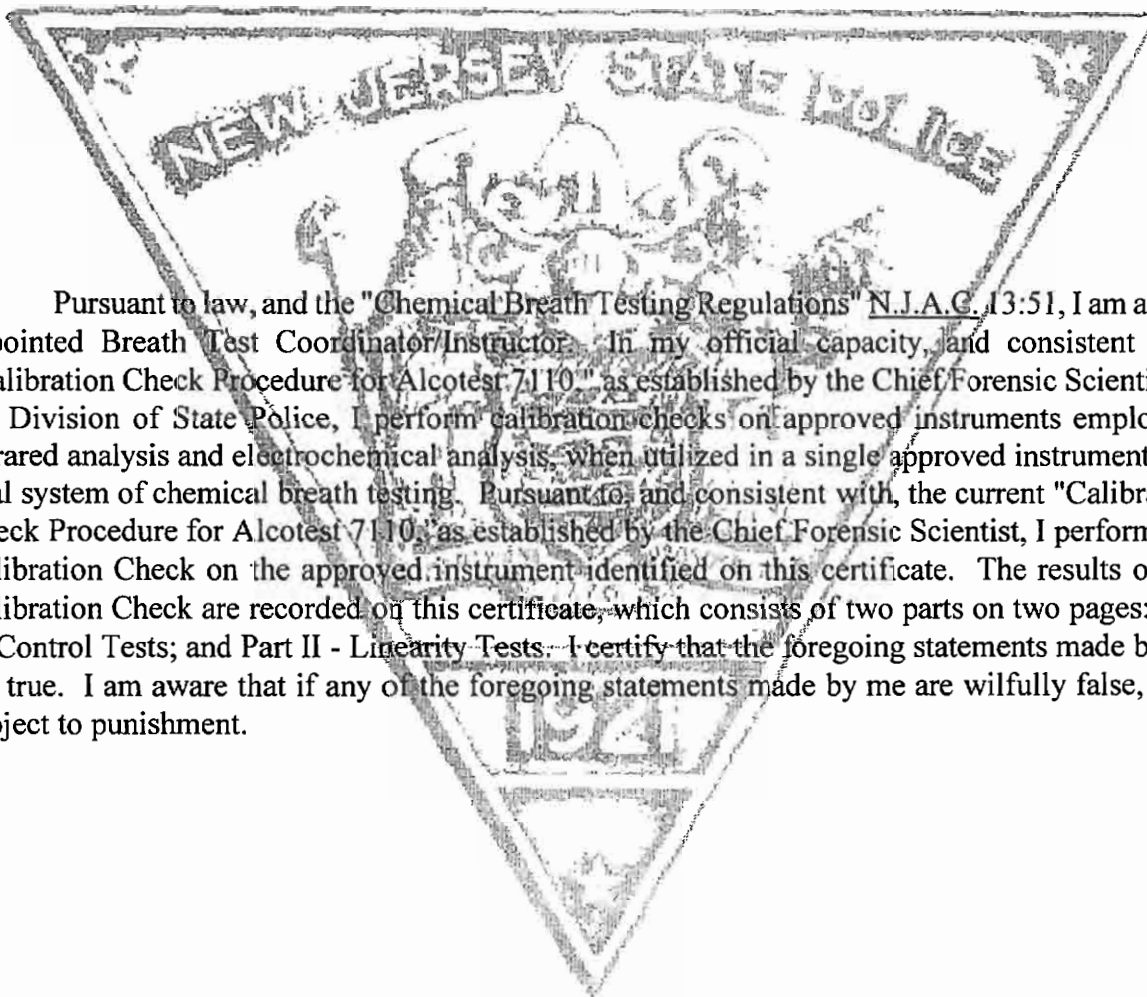

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
**Location:** BUENA BOROUGH POLICE  
**Calibration File No.:** 00004 **Calib. Date:** 11/05/2008 **Calib. No.:** 00002  
**Certification File No.:** 00005 **Cert. Date:** 11/05/2008 **Cert. No.:** 00001  
**Linearity File No.:** 00000 **Lin. Date:** --/--/---- **Lin. No.:** 00000  
**Solution File No.:** 00002 **Soln. Date:** 08/04/2006 **Soln. No.:** 00001  
**Sequential File No.:** 00005 **File Date:** 11/05/2008

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDXJ S3-0209  
**Control Solution %:** 0.100% **Expires:** 02/22/2009  
**Solution Control Lot:** 07B045 **Bottle No.:** 0367

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:28S		
Control 1 EC	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29S		
Control 2 EC	0.097%	09:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 3 EC	0.097%	09:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		

All tests within acceptable tolerance.

### Coordinator

Last Name: STANKS

First Name: ADAM

MI: N

Signature:

TPR. I Adam N. Stanks #5403

Badge No.: 5403

Date: 11/05/2008

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXB-0074  
**Location:** BUENA BOROUGH POLICE  
**Calibration File No.:** 00004 **Calib. Date:** 11/05/2008 **Calib. No.:** 00002  
**Certification File No.:** 00005 **Cert. Date:** 11/05/2008 **Cert. No.:** 00001  
**Linearity File No.:** 00006 **Lin. Date:** 11/05/2008 **Lin. No.:** 00001  
**Solution File No.:** 00002 **Soln. Date:** 08/04/2006 **Soln. No.:** 00001  
**Sequential File No.:** 00006 **File Date:** 11/05/2008

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0221  
**Control Solution %:** 0.040% **Expires:** 01/26/2009  
**Solution Control Lot:** 07A041 **Bottle No.:** 0386

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0223  
**Control Solution %:** 0.080% **Expires:** 01/26/2009  
**Solution Control Lot:** 07A042 **Bottle No.:** 0356

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDWF S3-0225  
**Control Solution %:** 0.160% **Expires:** 01/26/2009  
**Solution Control Lot:** 07A043 **Bottle No.:** 0178

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:49S		
Control 1 EC	0.040%	09:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		
Control 2 EC	0.039%	09:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.038%	09:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53S		
Control 3 EC	0.080%	09:54S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55S		
Control 4 EC	0.079%	09:55S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		
Control 5 EC	0.159%	09:57S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.162%	09:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59S		
Control 6 EC	0.159%	09:59S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.160%	09:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:01S		

All tests within acceptable tolerance.

### Coordinator

Last Name: STANKS

First Name: ADAM

MI: N

Signature: TPR. I Adam N. Stanks #5403

Badge No.: 5403

Date: 11/05/2008

DEPARTMENT OF  
**Law and Public Safety**  
This is to certify that

**ADAM N. STANKS**  
**NEW JERSEY STATE POLICE**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIIC**

A METHOD TO DETERMINE INTOXICATION.  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF December

TWO THOUSAND AND **FOUR**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	11/21/06	Sayreville PD	S. J. [Signature]
2.	2-2-08	CADAMY PA.	JC [Signature]
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 293B (Rev. 06/03)

DEPARTMENT OF  
**Law and Public Safety**  
This is to certify that

**Adam N. Stanks**  
**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE **Breathalyzer** METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF Apr.  
ONE THOUSAND NINE HUNDRED AND 97

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	4-26-88	ACTC	[Signature]
2.	10/12/01	OCPA	[Signature]
3.	9-3-03	ACTC	[Signature]
4.	7-18-05	ACTC	[Signature]
5.	3-2-07	OCPA	[Signature]
6.			
7.			
8.			
9.			

SP-293B



**Dräger**safety

**ALCOTEST® 7110 TEMPERATURE PROBE**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-024

Certification date:

08-25-08

Next Certification due:

08-25-09

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

JS



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

RON S. CORZINE  
 Governor

STUART RABNER  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A041

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.


As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

Notary

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

STUART RABNER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

JON S. CORZINE  
Governor

**CERTIFICATION OF ANALYSIS**  
**0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.

**ANALYSIS DATE:** 03/06/07

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 07A042

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0965 to 0.0972 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

  
Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





JON S. CORZINE  
Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

STUART RABNER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.

**ANALYSIS DATE:** 04/04/07

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 07B045

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 22, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 20<sup>th</sup> day of April, 2007.

Notary

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE

POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

STUART RABNER  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

JON S. CORZINE  
Governor

**CERTIFICATION OF ANALYSIS**  
**0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 03/06/07

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 07A043

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1932 to 0.1938 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.


As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Linda L. DeSantis  
My Commission  
Expires Aug. 17, 2008

*Ajit R. Tungare*  
Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police


Sworn to and subscribed before me this 29<sup>th</sup> day of March, 2007.

*Linda L. DeSantis*  
Notary



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWFS3-0221

Certification Date

Technician

Re-Certification Due Date

08-26-08

J.S.

08-26-09



**Draeger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWFS3-0223

Certification Date


Technician

Re-Certification Due Date

08-26-08

*AS*

08-26-09



Draeger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWFS3-0225

Certification Date

Technician

Re-Certification Due Date

08-26-08

AS

08-26-09



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXB-0074
<b>Location:</b>	BUENA BOROUGH POLICE		
<b>Calibration File No.:</b>	00004	<b>Calib. Date:</b>	11/05/2008
<b>Certification File No.:</b>	00005	<b>Cert. Date:</b>	11/05/2008
<b>Linearity File No.:</b>	00006	<b>Lin. Date:</b>	11/05/2008
<b>Solution File No.:</b>	00007	<b>Soln. Date:</b>	11/05/2008
<b>Sequential File No.:</b>	00007	<b>File Date:</b>	11/05/2008
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b>	CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b>	DDXJ S3-0209
<b>Solution Control Lot:</b>	08B050	<b>Expires:</b>	02/13/2010
		<b>Bottle No.:</b>	0477

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:09S		
Control 1 EC	0.101%	11:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10S		
Control 2 EC	0.099%	11:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:11S		
Control 3 EC	0.099%	11:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWAP2-148 *AMS*

**Changed By:**

Last Name: STANKS	First Name: ADAM	MI: N
Signature: <u><i>TPR. I Adam M. Stank #5403</i></u>	Badge No.: 5403	Date: 11/05/2008



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Dräger Safety, Inc.      **ANALYSIS DATE:** 03/14/2008

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 08B050

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1229 to 0.1234 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 13, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Ajit R. Tungare*  
 Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 31 <sup>st</sup> day of March, 2008.

*Linda L. DeSantis*

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable

