

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00655	Calib. Date: 12/17/2013
Certification File No.:	00656	Cert. No.: 00023
Linearity File No.:	00657	Cert. Date: 12/17/2013
Solution File No.:	00665	Lin. No.: 00016
Sequential File No.:	00665	Lin. Date: 12/17/2013
		Soln. No.: 00145
		Soln. Date: 12/31/2013
		File Date: 12/31/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1093

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:06S		
Control 1 EC	0.097%	06:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:07S		
Control 2 EC	0.096%	06:08S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:09S		
Control 3 EC	0.098%	06:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____

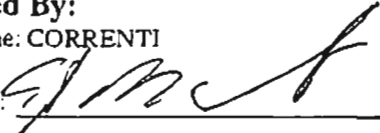

Badge No.: 4025

Date: 12/31/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053		
Location:	FLORENCE TOWNSHIP P.D.				
Calibration File No.:	00627	Calib. Date:	07/03/2013	Calib. No.:	00022
Certification File No.:	00628	Cert. Date:	07/03/2013	Cert. No.:	00015
Linearity File No.:	00629	Lin. Date:	07/03/2013	Lin. No.:	00015
Solution File No.:	00652	Soln. Date:	11/16/2013	Soln. No.:	00143
Sequential File No.:	00652	File Date:	11/16/2013		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	11/05/2014
Solution Control Lot:	12K108			Bottle No.:	1077

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:05S		
Control 1 EC	0.101%	21:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:06S		
Control 2 EC	0.099%	21:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:08S		
Control 3 EC	0.099%	21:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature:

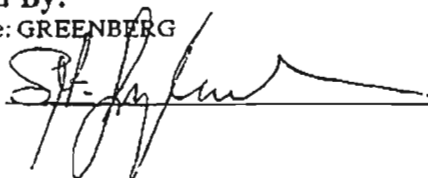

Badge No.: 4031

Date: 11/16/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKJII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00627	Calib. Date: 07/03/2013
Certification File No.:	00628	Cert. No.: 00015
Linearity File No.:	00629	Lin. Date: 07/03/2013
Solution File No.:	00647	Soln. No.: 00142
Sequential File No.:	00647	File Date: 10/19/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1089

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:04D		
Control 1 EC	0.099%	17:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:06D		
Control 2 EC	0.099%	17:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07D		
Control 3 EC	0.099%	17:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: _____

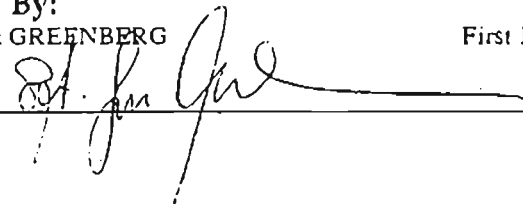

Badge No.: 4031

Date: 10/19/2013

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00627	Calib. Date: 07/03/2013
Certification File No.:	00628	Calib. No.: 00022
Linearity File No.:	00629	Cert. Date: 07/03/2013
Solution File No.:	00642	Cert. No.: 00015
Sequential File No.:	00642	Lin. Date: 07/03/2013
		Lin. No.: 00015
		Soln. Date: 09/18/2013
		Soln. No.: 00141
		File Date: 09/18/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1083

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:30D		
Control 1 EC	0.100%	04:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:31D		
Control 2 EC	0.100%	04:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:33D		
Control 3 EC	0.100%	04:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: _____

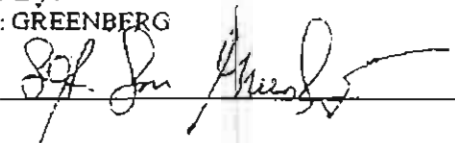

Badge No.: 4031

Date: 09/18/2013

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00627	Calib. Date: 07/03/2013
Certification File No.:	00628	Cert. No.: 00022
Linearity File No.:	00629	Cert. Date: 07/03/2013
Solution File No.:	00634	Lin. No.: 00015
Sequential File No.:	00634	Soln. No.: 00140
		File Date: 08/24/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1088

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:15D		
Control 1 EC	0.100%	00:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:16D		
Control 2 EC	0.099%	00:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:17D		
Control 3 EC	0.099%	00:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____



Badge No.: 4025

Date: 08/24/2013

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00627	Calib. Date: 07/03/2013
Certification File No.:	00628	Calib. No.: 00022
Linearity File No.:	00629	Cert. Date: 07/03/2013
Solution File No.:	00632	Cert. No.: 00015
Sequential File No.:	00632	Lin. Date: 07/03/2013
		Lin. No.: 00015
		Soln. Date: 07/24/2013
		Soln. No.: 00139
		File Date: 07/24/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %:	0.100%		Expires: 11/05/2014
Solution Control Lot:	12K108		Bottle No.: 1078

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:26D		
Control 1 EC	0.099%	07:27D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	07:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:28D		
Control 2 EC	0.098%	07:28D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:29D		
Control 3 EC	0.097%	07:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:30D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSF) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JONATHAN

MI: M

Signature: _____

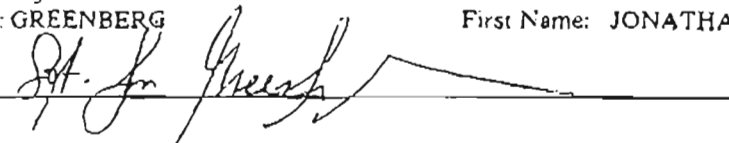

Badge No.: 4031

Date: 07/24/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00606	Calib. Date: 02/20/2013
Certification File No.:	00607	Calib. No.: 00021
Linearity File No.:	00608	Cert. Date: 02/20/2013
Solution File No.:	00622	Cert. No.: 00014
Sequential File No.:	00622	Lin. Date: 02/20/2013
		Lin. No.: 00014
		Soln. Date: 05/25/2013
		Soln. No.: 00136
		File Date: 05/25/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1080

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:12D		
Control 1 EC	0.101%	06:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13D		
Control 2 EC	0.100%	06:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:14D		
Control 3 EC	0.100%	06:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: _____

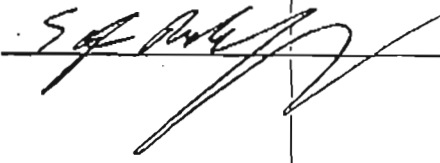

Badge No.: 4034

Date: 05/25/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00606	Calib. Date: 02/20/2013
Certification File No.:	00607	Calib. No.: 00021
Linearity File No.:	00608	Cert. Date: 02/20/2013
Solution File No.:	00621	Cert. No.: 00014
Sequential File No.:	00621	Lin. Date: 02/20/2013
		Lin. No.: 00014
		Soln. Date: 04/20/2013
		Soln. No.: 00135
		File Date: 04/20/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	12K108	Expires: 11/05/2014
		Bottle No.: 1090

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:57D		
Control 1 EC	0.101%	05:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	05:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:58D		
Control 2 EC	0.100%	05:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:00D		
Control 3 EC	0.100%	06:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: GREENBERG

First Name: JON

M1: M

Signature: _____

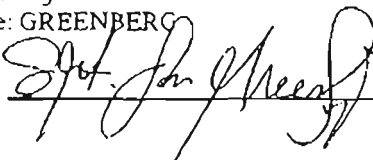

Badge No.: 4031

Date: 04/20/2013

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00606 **Calib. Date:** 02/20/2013 **Calib. No.:** 00021
Certification File No.: 00607 **Cert. Date:** 02/20/2013 **Cert. No.:** 00014
Linearity File No.: 00608 **Lin. Date:** 02/20/2013 **Lin. No.:** 00014
Solution File No.: 00615 **Soln. Date:** 03/25/2013 **Soln. No.:** 00134
Sequential File No.: 00615 **File Date:** 03/25/2013

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 11/05/2014
Solution Control Lot: 12K108 **Bottle No.:** 1100

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:01S		
Control 1 EC	0.100%	03:01S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:02S		
Control 2 EC	0.099%	03:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	03:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:03S		
Control 3 EC	0.099%	03:04S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 03/25/2013