

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWC-0060
Location: WILLINGBORO TWP POLICE
Calibration File No.: 00488 Calib. Date: 07/31/2014 Calib. No.: 00027
Certification File No.: 00489 Cert. Date: 07/31/2014 Cert. No.: 00020
Linearity File No.: 00490 Lin. Date: 07/31/2014 Lin. No.: 00020
Solution File No.: 00498 Soln. Date: 12/15/2014 Soln. No.: 00132
Sequential File No.: 00498 File Date: 12/15/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0189
Control Solution %: 0.100% Expires: 07/18/2015
Solution Control Lot: 13G115 Bottle No.: 0343

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:56S		
Control 1 EC	0.100%	10:57S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:57S		
Control 2 EC	0.101%	10:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59S		
Control 3 EC	0.100%	10:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____



Badge No.: 16187

Date: 12/15/2014



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWE 53-0189

Certification Date

Technician

Re-Certification Due Date

10-8-14

BC

10-8-15

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUN P2-293

10-6-14

10-6-15

Probe Value

104

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0060
Location:	WILLINGBORO TWP POLICE	
Calibration File No.:	00488	Calib. Date: 07/31/2014
Certification File No.:	00489	Calib. No.: 00027
Linearity File No.:	00490	Cert. Date: 07/31/2014
Solution File No.:	00496	Cert. No.: 00020
Sequential File No.:	00496	Lin. Date: 07/31/2014
		Lin. No.: 00020
		Soln. Date: 10/24/2014
		Soln. No.: 00130
		File Date: 10/24/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0188
Solution Control Lot:	13G115	Expires: 07/18/2015
		Bottle No.: 0347

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:28D		
Control 1 EC	0.100%	23:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	23:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:30D		
Control 2 EC	0.100%	23:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:31D		
Control 3 EC	0.100%	23:32D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	23:32D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____



Badge No.: 16187

Date: 10/24/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060		
Location:	WILLINGBORO TWP POLICE				
Calibration File No.:	00488	Calib. Date:	07/31/2014	Calib. No.:	00027
Certification File No.:	00489	Cert. Date:	07/31/2014	Cert. No.:	00020
Linearity File No.:	00490	Lin. Date:	07/31/2014	Lin. No.:	00020
Solution File No.:	00494	Soln. Date:	09/24/2014	Soln. No.:	00129
Sequential File No.:	00494	File Date:	09/24/2014		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWE S3-0188
Control Solution %:	0.100%			Expires:	07/18/2015
Solution Control Lot:	13G115			Bottle No.:	0346

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:16D		
Control 1 EC	0.101%	18:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:17D		
Control 2 EC	0.099%	18:18D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:18D		
Control 3 EC	0.099%	18:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: 

Badge No.: 16187

Date: 09/24/2014

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWC-0060
Location: WILLINGBORO TWP POLICE
Calibration File No.: 00488 Calib. Date: 07/31/2014 Calib. No.: 00027
Certification File No.: 00489 Cert. Date: 07/31/2014 Cert. No.: 00020
Linearity File No.: 00490 Lin. Date: 07/31/2014 Lin. No.: 00020
Solution File No.: 00493 Soln. Date: 08/27/2014 Soln. No.: 00128
Sequential File No.: 00493 File Date: 08/27/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0188
Control Solution %: 0.100% Expires: 07/18/2015
Solution Control Lot: 13G115 Bottle No.: 0334

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:46D		
Control 1 EC	0.099%	06:46D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:47D		
Control 2 EC	0.100%	06:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:48D		
Control 3 EC	0.099%	06:49D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____



Badge No.: 16187

Date: 08/27/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00469	Calib. Date:	02/19/2014
Certification File No.:	00470	Cert. Date:	02/19/2014
Linearity File No.:	00471	Lin. Date:	02/19/2014
Solution File No.:	00486	Soln. Date:	06/20/2014
Sequential File No.:	00486	File Date:	06/20/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE S3-0188
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	0335

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:56D		
Control 1 EC	0.098%	19:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:57D		
Control 2 EC	0.097%	19:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:59D		
Control 3 EC	0.098%	19:59D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____



Badge No.: 16187

Date: 06/20/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00469	Calib. Date:	02/19/2014
Certification File No.:	00470	Cert. No.:	00026
Linearity File No.:	00471	Calib. Date:	02/19/2014
Solution File No.:	00479	Cert. No.:	00019
Sequential File No.:	00479	Lin. Date:	02/19/2014
		Soln. Date:	05/19/2014
		Soln. No.:	00124
		File Date:	05/19/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE S3-0188
Solution Control Lot:	1303115	Expires:	07/18/2015
		Bottle No.:	8339

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:45D		
Control 1 BC	0.098%	21:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:47D		
Control 2 EC	0.099%	21:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48D		
Control 3 EC	0.099%	21:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____



Badge No.: 16187

Date: 05/19/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00469	Calib. Date:	02/19/2014
Certification File No.:	00470	Cert. Date:	02/19/2014
Linearity File No.:	00471	Lin. Date:	02/19/2014
Solution File No.:	00475	Soln. Date:	04/17/2014
Sequential File No.:	00475	File Date:	04/17/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE 53-0188
Solution Control Lot:	136115	Expires:	07/18/2015
		Bottle No.:	0340

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:01D		
Control 1 EC	0.098%	04:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:03D		
Control 2 EC	0.099%	04:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:04D		
Control 3 EC	0.099%	04:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NYS) Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____

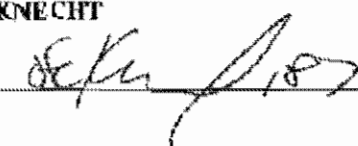

Badge No.: 16187

Date: 04/17/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00469	Calib. Date:	02/19/2014
Calibration File No.:	00470	Cert. No.:	00019
Linearity File No.:	00471	Lin. Date:	02/19/2014
Solution File No.:	00474	Soln. No.:	00122
Sequential File No.:	00474	File Date:	03/19/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DJWBK S1-0198
Solution Control Lot:	130115	Expires:	07/18/2015
		Bottle No.:	0350

Function	Result	Time	Temperature Simulator (°C)	Comments(s) or Pass(s)
Ambient Air Blank	0.000%	19:27S		
Control 1 EC	0.102%	19:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:25S		
Control 2 EC	0.101%	19:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:30S		
Control 3 EC	0.101%	19:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the [NISP] Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____

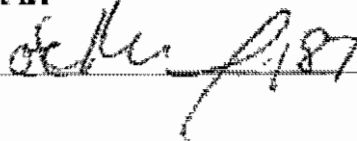

Badge No : 16187

Date: 03/19/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00469	Calib. Date:	02/19/2014
Certification File No.:	00470	Cert. Date:	02/19/2014
Linearity File No.:	00471	Lin. Date:	02/19/2014
Solution File No.:	00472	Soln. Date:	02/19/2014
Sequential File No.:	00472	File Date:	02/19/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE S3-0188
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	0341

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:12S		
Control 1 EC	0.100%	11:13S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13S		
Control 2 EC	0.100%	11:14S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15S		
Control 3 EC	0.100%	11:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUNP2-389 W01

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: A/Sgt. [Handwritten Signature] #6040

Badge No.: 6040

Date: 02/19/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKII-C	Serial No.:	ARWC-0060
Location:	WILLINGBORO TWP POLICE		
Calibration File No.:	00454	Calib. Date:	09/09/2013
Certification File No.:	00455	Cert. Date:	09/09/2013
Linearity File No.:	00456	Lin. Date:	09/09/2013
Solution File No.:	00465	Soln. Date:	01/09/2014
Sequential File No.:	00465	File Date:	01/09/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE SI-0188
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	0337

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:28S		
Control 1 EC	0.099%	20:29S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:29S		
Control 2 EC	0.099%	20:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:31S		
Control 3 EC	0.099%	20:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KNECHT

First Name: JENNIFER

MI: A

Signature: _____

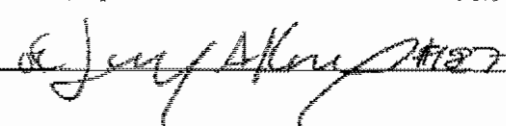

Badge No.: 16187

Date: 01/09/2014