

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00704 **Calib. Date:** 06/12/2014 **Calib. No.:** 00024  
**Certification File No.:** 00705 **Cert. Date:** 06/12/2014 **Cert. No.:** 00017  
**Linearity File No.:** 00706 **Lin. Date:** 06/12/2014 **Lin. No.:** 00017  
**Solution File No.:** 00738 **Soln. Date:** 10/10/2014 **Soln. No.:** 00157  
**Sequential File No.:** 00738 **File Date:** 10/10/2014

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222  
**Control Solution %:** 0.100% **Expires:** 04/29/2016  
**Solution Control Lot:** 14D129 **Bottle No.:** 0496

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 18:49D        |                               |                           |
| Control 1 EC      | 0.100%         | 18:49D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.099%         | 18:49D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 18:50D        |                               |                           |
| Control 2 EC      | 0.099%         | 18:51D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.100%         | 18:51D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 18:51D        |                               |                           |
| Control 3 EC      | 0.099%         | 18:52D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.101%         | 18:52D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 18:53D        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

M1: J

Signature: 

Badge No.: 4025

Date: 10/10/2014

# Calibrating Unit New Standard Solution Report

|                         |                        |                          |
|-------------------------|------------------------|--------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARTN-0053    |
| Location:               | FLORENCE TOWNSHIP P.D. |                          |
| Calibration File No.:   | 00704                  | Calib. Date: 06/12/2014  |
| Certification File No.: | 00705                  | Calib. No.: 00024        |
| Linearity File No.:     | 00706                  | Cert. Date: 06/12/2014   |
| Solution File No.:      | 00729                  | Cert. No.: 00017         |
| Sequential File No.:    | 00729                  | Lin. Date: 06/12/2014    |
|                         |                        | Lin. No.: 00017          |
|                         |                        | Soln. Date: 09/05/2014   |
|                         |                        | Soln. No.: 00156         |
|                         |                        | File Date: 09/05/2014    |
| Calibrating Unit:       | WET                    | Model No.: CU-34         |
| Control Solution %:     | 0.100%                 | Serial No.: DDUM S3-0222 |
| Solution Control Lot:   | 12K108                 | Expires: 11/05/2014      |
|                         |                        | Bottle No.: 1097         |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 08:28D |                |                     |
| Control 1 EC      | 0.098% | 08:29D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.097% | 08:29D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:30D |                |                     |
| Control 2 EC      | 0.097% | 08:30D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 08:30D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:31D |                |                     |
| Control 3 EC      | 0.098% | 08:32D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.098% | 08:32D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 08:32D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: LEVACH

First Name: CHARLES

MI: E

Signature: 

Badge No.: 4029

Date: 09/05/2014

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00704 **Calib. Date:** 06/12/2014 **Calib. No.:** 00024  
**Certification File No.:** 00705 **Cert. Date:** 06/12/2014 **Cert. No.:** 00017  
**Linearity File No.:** 00706 **Lin. Date:** 06/12/2014 **Lin. No.:** 00017  
**Solution File No.:** 00722 **Soln. Date:** 08/19/2014 **Soln. No.:** 00155  
**Sequential File No.:** 00722 **File Date:** 08/19/2014

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222  
**Control Solution %:** 0.100% **Expires:** 11/05/2014  
**Solution Control Lot:** 12K108 **Bottle No.:** 1096

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 08:59D |                |                     |
| Control 1 EC      | 0.096% | 09:00D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.096% | 09:00D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:01D |                |                     |
| Control 2 EC      | 0.097% | 09:01D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 09:01D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:02D |                |                     |
| Control 3 EC      | 0.096% | 09:02D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.098% | 09:02D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:03D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: 

Badge No.: 4034

Date: 08/19/2014

# Calibrating Unit New Standard Solution Report

|                          |                        |                          |
|--------------------------|------------------------|--------------------------|
| <b>Equipment</b>         | Alcotest 7110 MKIII-C  | Serial No.: ARTN-0053    |
| Location:                | FLORENCE TOWNSHIP P.D. |                          |
| Calibration File No.:    | 00704                  | Calib. Date: 06/12/2014  |
| Certification File No.:  | 00705                  | Cert. No.: 00024         |
| Linearity File No.:      | 00706                  | Cert. No.: 00017         |
| Solution File No.:       | 00717                  | Lin. Date: 06/12/2014    |
| Sequential File No.:     | 00717                  | Lin. No.: 00017          |
|                          |                        | Soln. No.: 00154         |
|                          |                        | Soln. Date: 07/19/2014   |
|                          |                        | File Date: 07/19/2014    |
| <b>Calibrating Unit:</b> | WET                    | Model No.: CU-34         |
| Control Solution %:      | 0.100%                 | Serial No.: DDUM S3-0222 |
| Solution Control Lot:    | 12K108                 | Expires: 11/05/2014      |
|                          |                        | Bottle No.: 1091         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 16:53D        |                               |                           |
| Control 1 EC      | 0.099%         | 16:53D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.098%         | 16:53D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 16:54D        |                               |                           |
| Control 2 EC      | 0.097%         | 16:55D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 16:55D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 16:55D        |                               |                           |
| Control 3 EC      | 0.097%         | 16:56D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.097%         | 16:56D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 16:56D        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4026

Date: 07/19/2014

# Calibrating Unit New Standard Solution Report

|                                |                        |                                 |
|--------------------------------|------------------------|---------------------------------|
| <b>Equipment</b>               | Alcotest 7110 MKIII-C  | Serial No.: ARTN-0053           |
| <b>Location:</b>               | FLORENCE TOWNSHIP P.D. |                                 |
| <b>Calibration File No.:</b>   | 00704                  | <b>Calib. Date:</b> 06/12/2014  |
| <b>Certification File No.:</b> | 00705                  | <b>Calib. No.:</b> 00024        |
| <b>Linearity File No.:</b>     | 00706                  | <b>Cert. Date:</b> 06/12/2014   |
| <b>Solution File No.:</b>      | 00711                  | <b>Cert. No.:</b> 00017         |
| <b>Sequential File No.:</b>    | 00711                  | <b>Lin. Date:</b> 06/12/2014    |
|                                |                        | <b>Lin. No.:</b> 00017          |
|                                |                        | <b>Soln. Date:</b> 06/22/2014   |
|                                |                        | <b>Soln. No.:</b> 00153         |
|                                |                        |                                 |
| <b>Calibrating Unit:</b>       | WET                    | <b>Model No.:</b> CU-34         |
| <b>Control Solution %:</b>     | 0.100%                 | <b>Serial No.:</b> DDUM S3-0222 |
| <b>Solution Control Lot:</b>   | 12K108                 | <b>Expires:</b> 11/05/2014      |
|                                |                        | <b>Bottle No.:</b> 1087         |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 07:30D |                |                     |
| Control 1 EC      | 0.098% | 07:30D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 07:30D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:31D |                |                     |
| Control 2 EC      | 0.096% | 07:31D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.097% | 07:31D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:32D |                |                     |
| Control 3 EC      | 0.097% | 07:33D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.098% | 07:33D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:33D |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 06/22/2014

# Calibrating Unit

## New Standard Solution Report

|                         |                        |                          |
|-------------------------|------------------------|--------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C  | Serial No.: ARTN-0053    |
| Location:               | FLORENCE TOWNSHIP P.D. |                          |
| Calibration File No.:   | 00655                  | Calib. Date: 12/17/2013  |
| Certification File No.: | 00656                  | Calib. No.: 00023        |
| Linearity File No.:     | 00657                  | Cert. Date: 12/17/2013   |
| Solution File No.:      | 00699                  | Cert. No.: 00016         |
| Sequential File No.:    | 00699                  | Lin. Date: 12/17/2013    |
|                         |                        | Lin. No.: 00016          |
|                         |                        | Soln. Date: 05/25/2014   |
|                         |                        | Soln. No.: 00151         |
|                         |                        | File Date: 05/25/2014    |
| <br>                    |                        |                          |
| Calibrating Unit:       | WET                    | Model No.: CU-34         |
| Control Solution %:     | 0.100%                 | Serial No.: DDUM S3-0225 |
| Solution Control Lot:   | 12K108                 | Expires: 11/05/2014      |
|                         |                        | Bottle No.: 1086         |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 04:37D |                |                     |
| Control 1 EC      | 0.097% | 04:37D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.097% | 04:37D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:38D |                |                     |
| Control 2 EC      | 0.097% | 04:39D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.097% | 04:39D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:39D |                |                     |
| Control 3 EC      | 0.097% | 04:40D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.097% | 04:40D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 04:41D |                |                     |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: YOUNG

First Name: BRIAN

MI: R

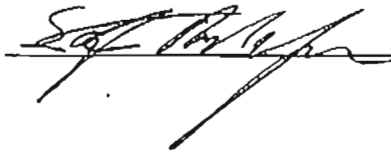Signature: 

Badge No.: 4034

Date: 05/25/2014

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
**Location:** FLORENCE TOWNSHIP P.D.  
**Calibration File No.:** 00655 **Calib. Date:** 12/17/2013 **Calib. No.:** 00023  
**Certification File No.:** 00656 **Cert. Date:** 12/17/2013 **Cert. No.:** 00016  
**Linearity File No.:** 00657 **Lin. Date:** 12/17/2013 **Lin. No.:** 00016  
**Solution File No.:** 00692 **Soln. Date:** 03/22/2014 **Soln. No.:** 00149  
**Sequential File No.:** 00692 **File Date:** 03/22/2014

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225  
**Control Solution %:** 0.100% **Expires:** 11/05/2014  
**Solution Control Lot:** 12K108 **Bottle No.:** 1081

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 01:54S        |                               |                           |
| Control 1 EC      | 0.098%         | 01:55S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.099%         | 01:55S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 01:56S        |                               |                           |
| Control 2 EC      | 0.096%         | 01:56S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.098%         | 01:56S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 01:57S        |                               |                           |
| Control 3 EC      | 0.096%         | 01:58S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.099%         | 01:58S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 01:59S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: \_\_\_\_\_



Badge No.: 4034

Date: 03/22/2014

# Calibrating Unit

## New Standard Solution Report

|                                |                        |                     |                                 |
|--------------------------------|------------------------|---------------------|---------------------------------|
| <b>Equipment</b>               | Alcotest 7110 MKIII-C  | Serial No.:         | ARTN-0053                       |
| <b>Location:</b>               | FLORENCE TOWNSHIP P.D. |                     |                                 |
| <b>Calibration File No.:</b>   | 00655                  | <b>Calib. Date:</b> | 12/17/2013                      |
| <b>Certification File No.:</b> | 00656                  | <b>Cert. Date:</b>  | 12/17/2013                      |
| <b>Linearity File No.:</b>     | 00657                  | <b>Lin. Date:</b>   | 12/17/2013                      |
| <b>Solution File No.:</b>      | 00686                  | <b>Soln. Date:</b>  | 02/25/2014                      |
| <b>Sequential File No.:</b>    | 00686                  | <b>File Date:</b>   | 02/25/2014                      |
| <br>                           |                        |                     |                                 |
| <b>Calibrating Unit:</b>       | WET                    | <b>Model No.:</b>   | CU-34                           |
| <b>Control Solution %:</b>     | 0.100%                 |                     | <b>Serial No.:</b> DDUM S3-0225 |
| <b>Solution Control Lot:</b>   | 12K108                 |                     | <b>Expires:</b> 11/05/2014      |
|                                |                        |                     | <b>Bottle No.:</b> 1099         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 14:47S        |                               |                           |
| Control 1 EC      | 0.099%         | 14:47S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.099%         | 14:47S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 14:48S        |                               |                           |
| Control 2 EC      | 0.097%         | 14:49S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 14:49S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 14:50S        |                               |                           |
| Control 3 EC      | 0.097%         | 14:50S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.097%         | 14:50S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 14:51S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: \_\_\_\_\_

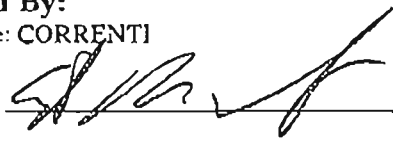

Badge No.: 4025

Date: 02/25/2014



# Calibrating Unit New Standard Solution Report

|                         |                        |             |            |
|-------------------------|------------------------|-------------|------------|
| Equipment               | Alcotest 7110 MKIII-C  | Serial No.: | ARTN-0053  |
| Location:               | FLORENCE TOWNSHIP P.D. | Calib. No.: | 00023      |
| Calibration File No.:   | 00655                  | Cert. Date: | 12/17/2013 |
| Certification File No.: | 00656                  | Calib. No.: | 00016      |
| Linearity File No.:     | 00657                  | Cert. No.:  | 00016      |
| Solution File No.:      | 00681                  | Lin. No.:   | 00016      |
| Sequential File No.:    | 00681                  | Soln. No.:  | 00147      |
|                         |                        | File Date:  | 02/11/2014 |

|                       |        |            |            |             |              |
|-----------------------|--------|------------|------------|-------------|--------------|
| Calibrating Unit:     | WET    | Model No.: | CU-34      | Serial No.: | DDUM S3-0225 |
| Control Solution %:   | 0.100% | Expires:   | 11/05/2014 | Bottle No.: | 1082         |
| Solution Control Lot: | 12K108 |            |            |             |              |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 22:08S |                |                     |
| Control 1 EC      | 0.099% | 22:09S | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.099% | 22:09S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:09S |                |                     |
| Control 2 EC      | 0.098% | 22:10S | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 22:10S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:11S |                |                     |
| Control 3 EC      | 0.098% | 22:12S | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.099% | 22:12S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 22:12S |                |                     |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 02/11/2014