

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00866 **Calib. Date:** 07/28/2016 **Calib. No.:** 00029
Certification File No.: 00867 **Cert. Date:** 07/28/2016 **Cert. No.:** 00022
Linearity File No.: 00868 **Lin. Date:** 07/28/2016 **Lin. No.:** 00022
Solution File No.: 00885 **Soln. Date:** 11/28/2016 **Soln. No.:** 00189
Sequential File No.: 00885 **File Date:** 11/28/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0222
Control Solution %: 0.100% **Expires:** 07/06/2018
Solution Control Lot: 16150 **Bottle No.:** 0884

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:20S		
Control 1 EC	0.100%	05:21S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	05:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21S		
Control 2 EC	0.099%	05:22S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:23S		
Control 3 EC	0.101%	05:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:24S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BONILLA

First Name: NICOLE

MI: M

Signature: 

Badge No.: 4043

Date: 11/28/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00866	Calib. Date: 07/28/2016
Certification File No.:	00867	Calib. No.: 00029
Linearity File No.:	00868	Cert. Date: 07/28/2016
Solution File No.:	00883	Cert. No.: 00022
Sequential File No.:	00883	Lin. Date: 07/28/2016
		Lin. No.: 00022
		Soln. Date: 10/27/2016
		Soln. No.: 00188
		File Date: 10/27/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0878

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:13D		
Control 1 EC	0.100%	02:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:15D		
Control 2 EC	0.099%	02:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:16D		
Control 3 EC	0.099%	02:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	02:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BONILLA

First Name: NICOLE

MI: M

Signature: _____



Badge No.: 4043

Date: 10/27/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00029
Calibration File No.:	00866	Calib. Date:	07/28/2016
Certification File No.:	00867	Cert. Date:	07/28/2016
Linearity File No.:	00868	Lin. Date:	07/28/2016
Solution File No.:	00878	Soln. Date:	09/24/2016
Sequential File No.:	00878	File Date:	09/24/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0222
Solution Control Lot:	201603L	Expires:	03/22/2018
		Bottle No.:	0451

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:35D		
Control 1 EC	0.102%	05:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	05:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:37D		
Control 2 EC	0.101%	05:37D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:38D		
Control 3 EC	0.101%	05:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	05:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:39D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____



Badge No.: 4041

Date: 09/24/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00866	Calib. Date: 07/28/2016
Certification File No.:	00867	Calib. No.: 00029
Linearity File No.:	00868	Cert. Date: 07/28/2016
Solution File No.:	00871	Cert. No.: 00022
Sequential File No.:	00871	Lin. Date: 07/28/2016
		Lin. No.: 00022
		Soln. Date: 08/25/2016
		Soln. No.: 00186
		File Date: 08/25/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0450

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:51D		
Control 1 EC	0.099%	15:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:52D		
Control 2 EC	0.098%	15:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:53D		
Control 3 EC	0.099%	15:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SADAR

First Name: TIMOTHY

MI: J

Signature:  #4035

Badge No.: 4035

Date: 08/25/2016

Signature:  #4035

Date: 08/25/2016

Signature:  #4035

Date: 08/25/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00845	Calib. Date: 03/08/2016
Certification File No.:	00846	Calib. No.: 00028
Linearity File No.:	00847	Cert. Date: 03/08/2016
Solution File No.:	00863	Lin. No.: 00021
Sequential File No.:	00863	Soln. Date: 07/15/2016
		Soln. No.: 00184
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0449

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:01D		
Control 1 EC	0.100%	21:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:03D		
Control 2 EC	0.099%	21:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	21:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:04D		
Control 3 EC	0.099%	21:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____



Badge No.: 4041

Date: 07/15/2016

Signature: _____



Date: 07/15/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00845	Calib. Date: 03/08/2016
Certification File No.:	00846	Cert. No.: 00028
Linearity File No.:	00847	Cert. Date: 03/08/2016
Solution File No.:	00859	Lin. No.: 00021
Sequential File No.:	00859	Lin. Date: 03/08/2016
		Soln. No.: 00183
		Soln. Date: 06/16/2016
		File Date: 06/16/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0452

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:59D		
Control 1 EC	0.105%	03:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:00D		
Control 2 EC	0.103%	04:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:01D		
Control 3 EC	0.102%	04:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	04:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:03D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:


Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: 

Badge No.: 4041
Date: 06/16/2016

Signature: 

Badge No.: 4041
Date: 06/16/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053		
Location:	FLORENCE TOWNSHIP P.D.				
Calibration File No.:	00845	Calib. Date:	03/08/2016	Calib. No.:	00028
Certification File No.:	00846	Cert. Date:	03/08/2016	Cert. No.:	00021
Linearity File No.:	00847	Lin. Date:	03/08/2016	Lin. No.:	00021
Solution File No.:	00855	Soln. Date:	05/06/2016	Soln. No.:	00181
Sequential File No.:	00855	File Date:	05/06/2016		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0222
Control Solution %:	0.100%			Expires:	01/05/2017
Solution Control Lot:	16A150			Bottle No.:	0925

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:46D		
Control 1 EC	0.102%	19:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:47D		
Control 2 EC	0.100%	19:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	19:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:49D		
Control 3 EC	0.100%	19:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:50D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B


Signature: _____



Badge No.: 4041

Date: 05/06/2016

Signature: _____



Badge No.: 4041

Date: 05/06/2016

Signature: _____



Badge No.: 4041

Date: 05/06/2016

Signature: _____



Badge No.: 4041

Date: 05/06/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00845	Calib. Date: 03/08/2016
Certification File No.:	00846	Cert. No.: 00028
Linearity File No.:	00847	Cert. Date: 03/08/2016
Solution File No.:	00854	Lin. Date: 03/08/2016
Sequential File No.:	00854	Lin. No.: 00021
		Soln. Date: 04/07/2016
		Soln. No.: 00180
		File Date: 04/07/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	16A150	Expires: 01/05/2017
		Bottle No.: 0919

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:33D		
Control 1 EC	0.101%	14:34D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:34D		
Control 2 EC	0.099%	14:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	14:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:36D		
Control 3 EC	0.100%	14:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:37D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:


Last Name: BOLDIZAR

First Name: BRIAN


MI: A

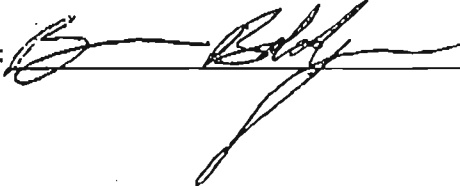Signature: 


Badge No.: 4001
Date: 04/07/2016

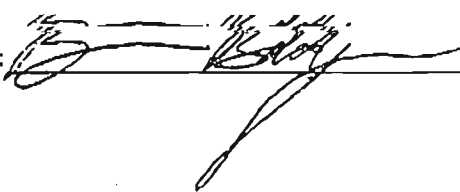Signature: 

Badge No.: 4001
Date: 04/07/2016

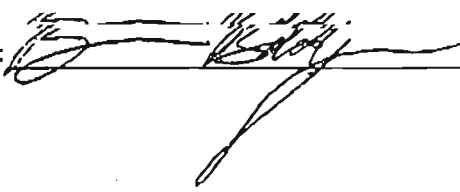Signature: 

Badge No.: 4001
Date: 04/07/2016

Signature: 

Badge No.: 4001
Date: 04/07/2016

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00818 **Calib. Date:** 10/13/2015 **Calib. No.:** 00027
Certification File No.: 00819 **Cert. Date:** 10/13/2015 **Cert. No.:** 00020
Linearity File No.: 00820 **Lin. Date:** 10/13/2015 **Lin. No.:** 00020
Solution File No.: 00844 **Soln. Date:** 03/01/2016 **Soln. No.:** 00178
Sequential File No.: 00844 **File Date:** 03/01/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 04/29/2016
Solution Control Lot: 14D129 **Bottle No.:** 0495

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:04S		
Control 1 EC	0.102%	03:05S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	03:05S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:06S		
Control 2 EC	0.099%	03:06S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.103%	03:06S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:07S		
Control 3 EC	0.100%	03:08S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	03:08S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: _____

Badge No.: 4034

Date: 03/01/2016

Signature: _____

Badge No.: 2037

Date: 03/01/2016

Solution File No.: 00844 **Soln. Date:** 03/01/2016 **Soln. No.:** 00178
Sequential File No.: 00844 **File Date:** 03/01/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 04/29/2016
Solution Control Lot: 14D129 **Bottle No.:** 0495

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:04S		

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00027
Calibration File No.:	00818	Calib. Date:	10/13/2015
Certification File No.:	00819	Cert. Date:	10/13/2015
Linearity File No.:	00820	Lin. Date:	10/13/2015
Solution File No.:	00840	Soln. Date:	02/01/2016
Sequential File No.:	00840	File Date:	02/01/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	0482

Function	Result - %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:04S		
Control 1 EC	0.101%	11:05S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:05S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		
Control 2 EC	0.100%	11:06S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.103%	11:06S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:07S		
Control 3 EC	0.100%	11:08S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.103%	11:08S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R


Signature: _____



Badge No.: 4034

Date: 02/01/2016


Signature: _____



Badge No.: 4034

Date: 02/01/2016


Signature: _____



Badge No.: 4034

Date: 02/01/2016

Signature: _____



Badge No.: 4034

Date: 02/01/2016

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00818 **Calib. Date:** 10/13/2015 **Calib. No.:** 00027
Certification File No.: 00819 **Cert. Date:** 10/13/2015 **Cert. No.:** 00020
Linearity File No.: 00820 **Lin. Date:** 10/13/2015 **Lin. No.:** 00020
Solution File No.: 00833 **Soln. Date:** 01/07/2016 **Soln. No.:** 00176
Sequential File No.: 00833 **File Date:** 01/07/2016

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 04/29/2016
Solution Control Lot: 14D129 **Bottle No.:** 0479


Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:46S		
Control 1 EC	0.103%	20:47S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.103%	20:47S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:48S		
Control 2 EC	0.101%	20:48S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.103%	20:48S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:49S		
Control 3 EC	0.101%	20:50S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.103%	20:50S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:51S		


All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CZEPIEL First Name: NICHOLAS MI: B
Signature:  Badge No.: 4041
Date: 01/07/2016

Last Name: CZEPIEL First Name: NICHOLAS MI: B
Signature:  Badge No.: 4041
Date: 01/07/2016

Last Name: CZEPIEL First Name: NICHOLAS MI: B
Signature:  Badge No.: 4041
Date: 01/07/2016

Last Name: CZEPIEL First Name: NICHOLAS MI: B
Signature:  Badge No.: 4041
Date: 01/07/2016