

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00951	Calib. Date: 11/08/2017
Certification File No.:	00952	Calib. No.: 00035
Linearity File No.:	00953	Cert. Date: 11/08/2017
Solution File No.:	00956	Cert. No.: 00027
Sequential File No.:	00956	Lin. Date: 11/08/2017
		Lin. No.: 00027
		Soln. Date: 12/07/2017
		Soln. No.: 00204
		File Date: 12/07/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUM S3-0222
Control Solution %:	0.100%		Expires: 03/20/2019
Solution Control Lot:	17110		Bottle No.: 1364

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:50S		
Control 1 EC	0.099%	04:51S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:51S		
Control 2 EC	0.098%	04:52S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:53S		
Control 3 EC	0.099%	04:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: 

Badge No.: 4025

Date: 12/07/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00951	Calib. Date: 11/08/2017
Certification File No.:	00952	Calib. No.: 00035
Linearity File No.:	00953	Cert. Date: 11/08/2017
Solution File No.:	00954	Cert. No.: 00027
Sequential File No.:	00954	Lin. Date: 11/08/2017
		Lin. No.: 00027
		Soln. Date: 11/08/2017
		Soln. No.: 00203
		File Date: 11/08/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	17110	Expires: 03/20/2019
		Bottle No.: 1353

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:49S		
Control 1 EC	0.101%	11:49S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50S		
Control 2 EC	0.100%	11:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		
Control 3 EC	0.099%	11:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJP2-293 MA

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Sgt. Michelle Gonalves #6040

Badge No.: 6040

Date: 11/08/2017

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00924	Calib. Date: 07/06/2017
Certification File No.:	00925	Calib. No.: 00034
Linearity File No.:	00926	Cert. Date: 07/06/2017
Solution File No.:	00948	Cert. No.: 00026
Sequential File No.:	00948	Lin. Date: 07/06/2017
		Lin. No.: 00026
		Soln. Date: 10/27/2017
		Soln. No.: 00202
		File Date: 10/27/2017

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %: 0.100%		Expires: 03/20/2019
Solution Control Lot: 17110		Bottle No.: 1344

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:24D		
Control 1 EC	0.103%	21:25D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	21:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:25D		
Control 2 EC	0.101%	21:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	21:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:27D		
Control 3 EC	0.101%	21:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____

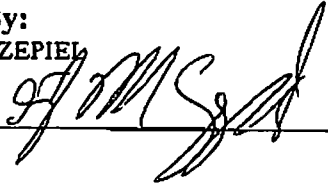

Badge No.: 4041

Date: 10/27/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00924	Calib. Date: 07/06/2017
Certification File No.:	00925	Calib. No.: 00034
Linearity File No.:	00926	Cert. Date: 07/06/2017
Solution File No.:	00946	Cert. No.: 00026
Sequential File No.:	00946	Lin. Date: 07/06/2017
		Lin. No.: 00026
		Soln. Date: 09/29/2017
		Soln. No.: 00201
		File Date: 09/29/2017

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %: 0.100%		Expires: 03/20/2019
Solution Control Lot: 17110		Bottle No.: 1334

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:14D		
Control 1 EC	0.103%	03:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	03:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:15D		
Control 2 EC	0.101%	03:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	03:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:16D		
Control 3 EC	0.101%	03:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	03:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____

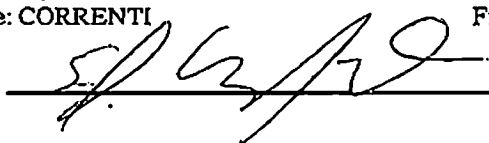

Badge No.: 4025

Date: 09/29/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	00924	Calib. Date:	07/06/2017
Certification File No.:	00925	Cert. No.:	00034
Linearity File No.:	00926	Cert. Date:	07/06/2017
Solution File No.:	00939	Lin. No.:	00026
Sequential File No.:	00939	Soln. Date:	08/31/2017
		Soln. No.:	00200
		File Date:	08/31/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	17110	Expires:	03/20/2019
		Bottle No.:	1325

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:14D		
Control 1 EC	0.102%	21:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	21:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:15D		
Control 2 EC	0.101%	21:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:16D		
Control 3 EC	0.100%	21:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	21:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____



Badge No.: 4041

Date: 08/31/2017

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00924 **Calib. Date:** 07/06/2017 **Calib. No.:** 00034
Certification File No.: 00925 **Cert. Date:** 07/06/2017 **Cert. No.:** 00026
Linearity File No.: 00926 **Lin. Date:** 07/06/2017 **Lin. No.:** 00026
Solution File No.: 00936 **Soln. Date:** 08/03/2017 **Soln. No.:** 00199
Sequential File No.: 00936 **File Date:** 08/03/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 03/20/2019
Solution Control Lot: 17110 **Bottle No.:** 1321

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:12D		
Control 1 EC	0.102%	01:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	01:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:13D		
Control 2 EC	0.101%	01:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	01:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 3 EC	0.102%	01:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	01:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCULLY

First Name: DANIEL

MI: S

Signature: 

Badge No.: 4065

Date: 08/03/2017

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00924	Calib. Date: 07/06/2017
Certification File No.:	00925	Calib. No.: 00034
Linearity File No.:	00926	Cert. No.: 00026
Solution File No.:	00929	Lin. No.: 00026
Sequential File No.:	00929	Soln. No.: 00198
		File Date: 07/07/2017

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUM S3-0225
Control Solution %: 0.100%		Expires: 07/06/2018
Solution Control Lot: 16150		Bottle No.: 0880

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:04D		
Control 1 EC	0.100%	01:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:05D		
Control 2 EC	0.099%	01:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:07D		
Control 3 EC	0.099%	01:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: YOUNG

First Name: BRIAN

MI: R

Signature: _____

Badge No.: 4034

Date: 07/07/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00896	Calib. Date: 01/20/2017
Certification File No.:	00897	Calib. No.: 00033
Linearity File No.:	00898	Cert. Date: 01/20/2017
Solution File No.:	00923	Cert. No.: 00025
Sequential File No.:	00923	Lin. Date: 01/20/2017
		Lin. No.: 00025
		Soln. Date: 07/03/2017
		Soln. No.: 00196
		File Date: 07/03/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0898

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:49D		
Control 1 EC	0.100%	04:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	04:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:50D		
Control 2 EC	0.098%	04:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:51D		
Control 3 EC	0.098%	04:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SCULLY

First Name: DANIEL

MI: S

Signature: _____



Badge No.: 4065

Date: 07/03/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00896	Calib. Date: 01/20/2017
Certification File No.:	00897	Calib. No.: 00033
Linearity File No.:	00898	Cert. Date: 01/20/2017
Solution File No.:	00919	Cert. No.: 00025
Sequential File No.:	00919	Lin. Date: 01/20/2017
		Lin. No.: 00025
		Soln. Date: 06/03/2017
		Soln. No.: 00195
		File Date: 06/03/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 1232

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:26D		
Control 1 EC	0.100%	08:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:27D		
Control 2 EC	0.099%	08:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:28D		
Control 3 EC	0.100%	08:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____

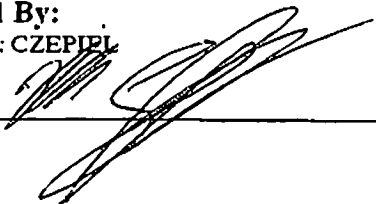

Badge No.: 4041

Date: 06/03/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00896	Calib. Date: 01/20/2017
Certification File No.:	00897	Calib. No.: 00033
Linearity File No.:	00898	Cert. Date: 01/20/2017
Solution File No.:	00913	Cert. No.: 00025
Sequential File No.:	00913	Lin. Date: 01/20/2017
		Lin. No.: 00025
		Soln. Date: 05/02/2017
		Soln. No.: 00194
		File Date: 05/02/2017
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 1229

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:02D		
Control 1 EC	0.100%	00:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:03D		
Control 2 EC	0.100%	00:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:04D		
Control 3 EC	0.100%	00:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CORRENTI

First Name: MAURO

MI: J

Signature: _____



Badge No.: 4025

Date: 05/02/2017

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	00896	Calib. Date: 01/20/2017
Certification File No.:	00897	Calib. No.: 00033
Linearity File No.:	00898	Cert. Date: 01/20/2017
Solution File No.:	00907	Cert. No.: 00025
Sequential File No.:	00907	Lin. Date: 01/20/2017
		Lin. No.: 00025
		Soln. Date: 04/01/2017
		Soln. No.: 00193
		File Date: 04/01/2017

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	16150	Expires: 07/06/2018
		Bottle No.: 0877

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:56S		
Control 1 EC	0.100%	02:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:57S		
Control 2 EC	0.099%	02:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:58S		
Control 3 EC	0.099%	02:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SHAFER

First Name: JASON

MI: A

Signature: _____



Badge No.: 4045

Date: 04/01/2017

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 00896 **Calib. Date:** 01/20/2017 **Calib. No.:** 00033
Certification File No.: 00897 **Cert. Date:** 01/20/2017 **Cert. No.:** 00025
Linearity File No.: 00898 **Lin. Date:** 01/20/2017 **Lin. No.:** 00025
Solution File No.: 00904 **Soln. Date:** 02/28/2017 **Soln. No.:** 00192
Sequential File No.: 00904 **File Date:** 02/28/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUM S3-0225
Control Solution %: 0.100% **Expires:** 07/06/2018
Solution Control Lot: 16150 **Bottle No.:** 1140

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:09S		
Control 1 EC	0.101%	08:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		
Control 2 EC	0.100%	08:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12S		
Control 3 EC	0.100%	08:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPJEL

First Name: NICHOLAS

MI: B

Signature: _____

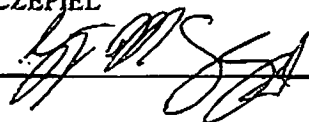

Badge No.: 4041

Date: 02/28/2017