

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01037	Calib. No.: 00039
Certification File No.:	01038	Cert. No.: 00031
Linearity File No.:	01039	Lin. No.: 00031
Solution File No.:	01064	Soln. No.: 00239
Sequential File No.:	01064	File Date: 12/04/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	19240	Expires: 09/09/2021
		Bottle No.: 0759

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:26S		
Control 1 EC	0.100%	06:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:27S		
Control 2 EC	0.098%	06:28S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:29S		
Control 3 EC	0.098%	06:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: \_\_\_\_\_



Badge No.: 4047

Date: 12/04/2019

# Calibrating Unit New Standard Solution Report



<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053		
Location:	FLORENCE TOWNSHIP P.D.				
Calibration File No.:	01037	Calib. Date:	07/09/2019	Calib. No.:	00039
Certification File No.:	01038	Cert. Date:	07/09/2019	Cert. No.:	00031
Linearity File No.:	01039	Lin. Date:	07/09/2019	Lin. No.:	00031
Solution File No.:	01063	Soln. Date:	11/09/2019	Soln. No.:	00238
Sequential File No.:	01063	File Date:	11/09/2019		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	09/09/2021
Solution Control Lot:	19240			Bottle No.:	0336

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:07S		
Control 1 EC	0.097%	19:08S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:08S		
Control 2 EC	0.096%	19:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:10S		
Control 3 EC	0.097%	19:10S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:10S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name:	YOUNG	First Name:	BRIAN	MI:	R
Signature:		Badge No.:	4034	Date:	11/09/2019
Signature:		Badge No.:	4034	Date:	11/09/2019

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053		
Location:	FLORENCE TOWNSHIP P.D.				
Calibration File No.:	01037	Calib. Date:	07/09/2019	Calib. No.:	00039
Certification File No.:	01038	Cert. Date:	07/09/2019	Cert. No.:	00031
Linearity File No.:	01039	Lin. Date:	07/09/2019	Lin. No.:	00031
Solution File No.:	01058	Soln. Date:	11/02/2019	Soln. No.:	00237
Sequential File No.:	01058	File Date:	11/02/2019		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	09/17/2020
Solution Control Lot:	18290			Bottle No.:	0068

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:38S		
Control 1 EC	0.098%	17:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	17:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:40S		
Control 2 EC	0.097%	17:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:41S		
Control 3 EC	0.096%	17:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI: J


Signature: \_\_\_\_\_



Badge No.: 4025

Date: 11/02/2019

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 11/02/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01037	Calib. Date:	07/09/2019
Certification File No.:	01038	Cert. Date:	07/09/2019
Linearity File No.:	01039	Lin. Date:	07/09/2019
Solution File No.:	01053	Soln. Date:	10/05/2019
Sequential File No.:	01053	File Date:	10/05/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	18290	Expires:	09/17/2020
		Bottle No.:	0609

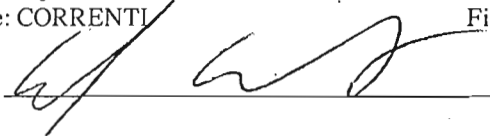
Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:16D		
Control 1 EC	0.099%	20:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	20:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:17D		
Control 2 EC	0.098%	20:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:19D		
Control 3 EC	0.098%	20:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:20D		


All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI First Name: MAURO MI: J

Signature:  Badge No.: 4025  
Date: 10/05/2019

Signature:  Badge No.: 4025  
Date: 10/05/2019

# Calibrating Unit

## New Standard Solution Report

### Equipment

Alcotest 7110 MKIII-C  
Location: FLORENCE TOWNSHIP P.D.  
Serial No.: ARTN-0053  
Calibration File No.: 01037 Calib. Date: 07/09/2019 Calib. No.: 00039  
Certification File No.: 01038 Cert. Date: 07/09/2019 Cert. No.: 00031  
Linearity File No.: 01039 Lin. Date: 07/09/2019 Lin. No.: 00031  
Solution File No.: 01052 Soln. Date: 09/09/2019 Soln. No.: 00235  
Sequential File No.: 01052 File Date: 09/09/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225  
Control Solution %: 0.100% Expires: 01/31/2020  
Solution Control Lot: 18050 Bottle No.: 1095

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:37D		
Control 1 EC	0.099%	01:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:38D		
Control 2 EC	0.099%	01:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:40D		
Control 3 EC	0.099%	01:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	01:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: \_\_\_\_\_



Badge No.: 4041

Date: 09/09/2019

Signature: \_\_\_\_\_



Badge No.: 4041

Date: 09/09/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01037	Calib. Date:	07/09/2019
Certification File No.:	01038	Cert. Date:	07/09/2019
Linearity File No.:	01039	Lin. Date:	07/09/2019
Solution File No.:	01046	Soln. Date:	08/27/2019
Sequential File No.:	01046	File Date:	08/27/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	18290	Expires:	09/17/2020
		Bottle No.:	0772

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:32D		
Control 1 EC	0.099%	02:33D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:33D		
Control 2 EC	0.097%	02:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:35D		
Control 3 EC	0.098%	02:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:36D		

All tests within acceptable tolerance.

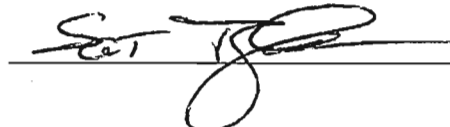
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

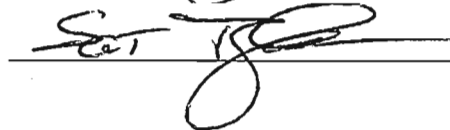
**Changed By:**

Last Name: SADAR

First Name: TIMOTHY

MI: J

Signature: 

Signature: 

Badge No.: 4035  
Date: 08/27/2019

Badge No.: 4035  
Date: 08/27/2019

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
 Location: FLORENCE TOWNSHIP P.D.  
 Calibration File No.: 01037 Calib. Date: 07/09/2019 Calib. No.: 00039  
 Certification File No.: 01038 Cert. Date: 07/09/2019 Cert. No.: 00031  
 Linearity File No.: 01039 Lin. Date: 07/09/2019 Lin. No.: 00031  
 Solution File No.: 01043 Soln. Date: 07/25/2019 Soln. No.: 00232  
 Sequential File No.: 01043 File Date: 07/25/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225  
 Control Solution %: 0.100% Expires: 09/17/2020  
 Solution Control Lot: 18290 Bottle No.: 0616

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:45D		
Control 1 EC	0.099%	09:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		
Control 2 EC	0.098%	09:47D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:47D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48D		
Control 3 EC	0.098%	09:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWI P2-144 (DW)

**Changed By:**

Last Name: NAPOLITANO First Name: DAVID MI: M.

Signature:  Badge No.: 7237  
Date: 07/25/2019

Signature:  Badge No.: 7237  
Date: 07/25/2019

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: \_\_\_\_\_

Serial Number:

DDUM53-0225

Certification Date:

Technician:

Re-Certification Due Date:

6-27-19

BS

6-27-20

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

ALCOTEST 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.  
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDW\p2-144

6-27-19

6-27-20

Probe Value:

99

Draeger, Inc.

BS



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01013	Calib. Date: 01/24/2019
Certification File No.:	01014	Calib. No.: 00038
Linearity File No.:	01015	Cert. Date: 01/24/2019
Solution File No.:	01033	Cert. No.: 00030
Sequential File No.:	01033	Lin. Date: 01/24/2019
		Lin. No.: 00030
		Soln. Date: 06/06/2019
		Soln. No.: 00230
		File Date: 06/06/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	18290	Expires: 09/17/2020
		Bottle No.: 0172

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:18D		
Control 1 EC	0.101%	11:19D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	11:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 2 EC	0.098%	11:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21D		
Control 3 EC	0.098%	11:21D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: CORRENTI

First Name: MAURO

MI:


Signature: \_\_\_\_\_



Badge No.: 4025

Date: 06/06/2019

Signature: \_\_\_\_\_



Badge No.: 4025

Date: 06/06/2019

# Calibrating Unit

## New Standard Solution Report



<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01013	Calib. Date: 01/24/2019      Calib. No.: 00038
Certification File No.:	01014	Cert. Date: 01/24/2019      Cert. No.: 00030
Linearity File No.:	01015	Lin. Date: 01/24/2019      Lin. No.: 00030
Solution File No.:	01032	Soln. Date: 05/09/2019      Soln. No.: 00229
Sequential File No.:	01032	File Date: 05/09/2019
Calibrating Unit:	WET	Model No.: CU-34      Serial No.: DDUM S3-0222
Control Solution %:	0.100%	Expires: 09/17/2020
Solution Control Lot:	18290	Bottle No.: 0131

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:19D		
Control 1 EC	0.101%	01:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:20D		
Control 2 EC	0.099%	01:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:21D		
Control 3 EC	0.099%	01:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CZEPIEL	First Name: NICHOLAS	MI: B
Signature: 		Badge No.: 4041
		Date: 05/09/2019
Signature: 		Badge No.: 4041
		Date: 05/09/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01013	Calib. Date:	01/24/2019
Certification File No.:	01014	Cert. No.:	00038
Linearity File No.:	01015	Cert. Date:	01/24/2019
Solution File No.:	01025	Lin. No.:	00030
Sequential File No.:	01025	Lin. Date:	01/24/2019
		Soln. No.:	00228
		Soln. Date:	04/04/2019
		File Date:	04/04/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0222
Control Solution %:	0.100%			Expires:	01/31/2020
Solution Control Lot:	18050			Bottle No.:	1340

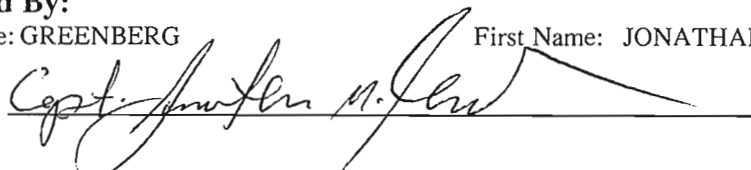
Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:56S		
Control 1 EC	0.100%	08:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57S		
Control 2 EC	0.099%	08:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59S		
Control 3 EC	0.098%	08:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:00S		

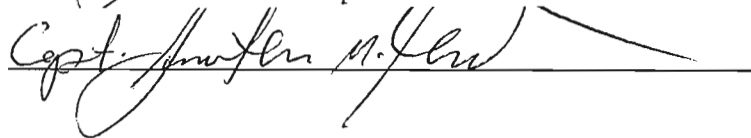
All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GREENBERG      First Name: JONATHAN      MI: M

Signature:  \_\_\_\_\_  
 Badge No.: 4031  
 Date: 04/04/2019

Signature:  \_\_\_\_\_  
 Badge No.: 4031  
 Date: 04/04/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01013	Calib. Date: 01/24/2019
Certification File No.:	01014	Calib. No.: 00038
Linearity File No.:	01015	Cert. Date: 01/24/2019
Solution File No.:	01024	Cert. No.: 00030
Sequential File No.:	01024	Lin. Date: 01/24/2019
		Lin. No.: 00030
		Soln. Date: 03/31/2019
		Soln. No.: 00227
		File Date: 03/31/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	18050	Expires: 01/31/2020
		Bottle No.: 1340

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:37S		
Control 1 EC	-.---%	23:38S	21.5°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	23:38S	21.5°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

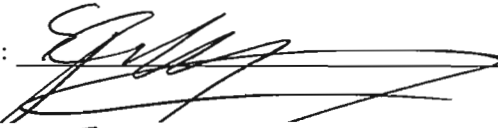
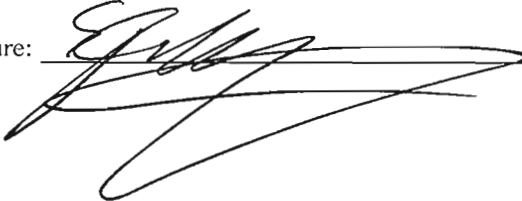
Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: YOUNG	First Name: BRIAN	MI: R
------------------	-------------------	-------

Signature: 	Badge No.: 4034
	Date: 03/31/2019
-----	
Signature: 	Badge No.: 4034
	Date: 03/31/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01013	Calib. Date: 01/24/2019
Certification File No.:	01014	Cert. No.: 00038
Linearity File No.:	01015	Cert. Date: 01/24/2019
Solution File No.:	01022	Lin. No.: 00030
Sequential File No.:	01022	Lin. Date: 01/24/2019
		Soln. No.: 00226
		Soln. Date: 03/26/2019
		File Date: 03/26/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	18290	Expires: 09/17/2020
		Bottle No.: 0980

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:02S		
Control 1 EC	0.099%	00:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:04S		
Control 2 EC	0.098%	00:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:05S		
Control 3 EC	0.097%	00:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**


Last Name: SCULLY

First Name: DANIEL

MI: S

Signature:  \_\_\_\_\_

Badge No.: 4065  
Date: 03/26/2019

Signature:  \_\_\_\_\_

Badge No.: 4065  
Date: 03/26/2019

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0053  
Location: FLORENCE TOWNSHIP P.D.  
Calibration File No.: 01013 Calib. Date: 01/24/2019 Calib. No.: 00038  
Certification File No.: 01014 Cert. Date: 01/24/2019 Cert. No.: 00030  
Linearity File No.: 01015 Lin. Date: 01/24/2019 Lin. No.: 00030  
Solution File No.: 01021 Soln. Date: 03/25/2019 Soln. No.: 00225  
Sequential File No.: 01021 File Date: 03/25/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0222  
Control Solution %: 0.100% Expires: 09/17/2020  
Solution Control Lot: 18290 Bottle No.: 0454

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:07S		
Control 1 EC	-.---%	01:08S	23.1°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	01:08S	23.1°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: \_\_\_\_\_



Badge No.: 4041

Date: 03/25/2019

Signature: \_\_\_\_\_



Badge No.: 4041

Date: 03/25/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01013	Calib. Date:	01/24/2019
Certification File No.:	01014	Cert. Date:	01/24/2019
Linearity File No.:	01015	Lin. Date:	01/24/2019
Solution File No.:	01019	Soln. Date:	03/14/2019
Sequential File No.:	01019	File Date:	03/14/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0222
Control Solution %:	0.100%			Expires:	01/31/2020
Solution Control Lot:	18050			Bottle No.:	1300

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:51S		
Control 1 EC	0.099%	00:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	00:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:53S		
Control 2 EC	0.098%	00:53S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:54S		
Control 3 EC	0.098%	00:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:55S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCULLY


First Name: DANIEL

MI: S

Signature:  \_\_\_\_\_

Badge No.: 4065

Date: 03/14/2019

Signature:  \_\_\_\_\_

Badge No.: 4065

Date: 03/14/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01013	Calib. Date: 01/24/2019
Certification File No.:	01014	Cert. No.: 00038
Linearity File No.:	01015	Cert. Date: 01/24/2019
Solution File No.:	01017	Lin. No.: 00030
Sequential File No.:	01017	Lin. Date: 01/24/2019
		Soln. No.: 00223
		Soln. Date: 02/13/2019
		File Date: 02/13/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	18290	Expires: 09/17/2020
		Bottle No.: 0018

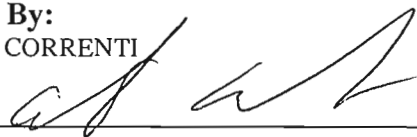
Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:25S		
Control 1 EC	0.099%	05:26S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:27S		
Control 2 EC	0.097%	05:27S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:27S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:28S		
Control 3 EC	0.097%	05:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:30S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: CORRENTI      First Name: MAURO      MI: J

Signature: 

Badge No.: 4025  
Date: 02/13/2019

Signature: 

Badge No.: 4025  
Date: 02/13/2019