

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01179	Calib. No.: 00048
Certification File No.:	01180	Cert. No.: 00040
Linearity File No.:	01181	Lin. No.: 00039
Solution File No.:	01205	Soln. No.: 00282
Sequential File No.:	01205	File Date: 11/10/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 0239

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:31S		
Control 1 EC	-.---%	15:31S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	15:31S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CZEPIEL

First Name: NICHOLAS

MI: B

Signature: _____

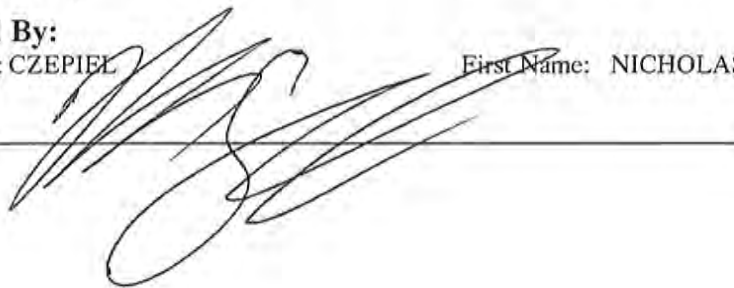

Badge No.: 4002

Date: 11/10/2022

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.		
Calibration File No.:	01179	Calib. Date:	07/06/2022
Certification File No.:	01180	Cert. Date:	07/06/2022
Linearity File No.:	01181	Lin. Date:	07/06/2022
Solution File No.:	01204	Soln. Date:	11/03/2022
Sequential File No.:	01204	File Date:	11/03/2022
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	22160	Expires:	05/09/2024
		Bottle No.:	0416

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:10S		
Control 1 EC	-.--%	05:10S	34.0°C	CTRL GAS SUPPLY CTRL GAS SUPPLY
Control 1 IR	-.--%	05:10S	34.0°C	
Ambient Air Blank	-.--%	--:--		
Control 2 EC	-.--%	--:--	N/A	
Control 2 IR	-.--%	--:--	N/A	
Ambient Air Blank	-.--%	--:--		
Control 3 EC	-.--%	--:--	N/A	
Control 3 IR	-.--%	--:--	N/A	
Ambient Air Blank	-.--%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LLOYD

First Name: MATTHEW

MI: T

Signature: _____

Badge No.: 4059

Date: 11/03/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00048
Calibration File No.:	01179	Cert. Date:	07/06/2022
Certification File No.:	01180	Lin. Date:	07/06/2022
Linearity File No.:	01181	Soln. Date:	10/31/2022
Solution File No.:	01203	File Date:	10/31/2022
Sequential File No.:	01203		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUM S3-0225
Solution Control Lot:	22160	Expires:	05/09/2024
		Bottle No.:	0418

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:12S		
Control 1 EC	-.---%	07:12S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	07:12S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 10/31/2022

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01179	Calib. Date: 07/06/2022
Certification File No.:	01180	Calib. No.: 00048
Linearity File No.:	01181	Cert. Date: 07/06/2022
Solution File No.:	01196	Cert. No.: 00040
Sequential File No.:	01196	Lin. Date: 07/06/2022
		Lin. No.: 00039
		Soln. Date: 10/02/2022
		Soln. No.: 00278
		File Date: 10/02/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	22110	Expires: 04/04/2024
		Bottle No.: 0657

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:41D		
Control 1 EC	0.103%	18:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	18:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:42D		
Control 2 EC	0.100%	18:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	18:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:44D		
Control 3 EC	0.101%	18:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	18:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILK

First Name: JASON

MI: J

Signature: _____



Badge No.: 4049

Date: 10/02/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01179	Calib. Date: 07/06/2022
Certification File No.:	01180	Calib. No.: 00048
Linearity File No.:	01181	Cert. Date: 07/06/2022
Solution File No.:	01190	Cert. No.: 00040
Sequential File No.:	01190	Lin. Date: 07/06/2022
		Lin. No.: 00039
		Soln. Date: 09/04/2022
		Soln. No.: 00277
		File Date: 09/04/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	22160	Expires: 05/09/2024
		Bottle No.: 0199

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:06D		
Control 1 EC	0.099%	04:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:07D		
Control 2 EC	0.100%	04:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:09D		
Control 3 EC	0.099%	04:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BONILLA

First Name: NICOLE

MI: M

Signature: _____



Badge No.: 4043

Date: 09/04/2022

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01179 Calib. Date: 07/06/2022 Calib. No.: 00048
Certification File No.: 01180 Cert. Date: 07/06/2022 Cert. No.: 00040
Linearity File No.: 01181 Lin. Date: 07/06/2022 Lin. No.: 00039
Solution File No.: 01185 Soln. Date: 08/04/2022 Soln. No.: 00276
Sequential File No.: 01185 File Date: 08/04/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 05/09/2024
Solution Control Lot: 22160 Bottle No.: 0598

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:58D		
Control 1 EC	0.101%	06:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:59D		
Control 2 EC	0.099%	06:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:00D		
Control 3 EC	0.100%	07:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SADAR

First Name: TIMOMTHY

MI: J

Signature: _____



Badge No.: 4035

Date: 08/04/2022

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01161 Calib. Date: 02/08/2022 Calib. No.: 00047
Certification File No.: 01162 Cert. Date: 02/08/2022 Cert. No.: 00039
Linearity File No.: 01163 Lin. Date: 02/08/2022 Lin. No.: 00038
Solution File No.: 01174 Soln. Date: 06/02/2022 Soln. No.: 00274
Sequential File No.: 01174 File Date: 06/02/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 02/17/2024
Solution Control Lot: 22070 Bottle No.: 1212

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:32D		
Control 1 EC	0.103%	07:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:34D		
Control 2 EC	0.101%	07:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:35D		
Control 3 EC	0.101%	07:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 06/02/2022

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	Calib. No.:	00047
Calibration File No.:	01161	Calib. Date:	02/08/2022
Certification File No.:	01162	Cert. Date:	02/08/2022
Linearity File No.:	01163	Lin. Date:	02/08/2022
Solution File No.:	01172	Soln. Date:	05/02/2022
Sequential File No.:	01172	File Date:	05/02/2022

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUM S3-0225
Control Solution %:	0.100%			Expires:	07/06/2022
Solution Control Lot:	20320			Bottle No.:	0337

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:16D		
Control 1 EC	0.100%	01:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:17D		
Control 2 EC	0.099%	01:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:19D		
Control 3 EC	0.098%	01:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____

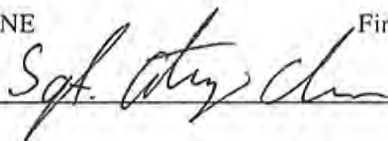

Badge No.: 4047

Date: 05/02/2022

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0053
Location: FLORENCE TOWNSHIP P.D.
Calibration File No.: 01161 Calib. Date: 02/08/2022 Calib. No.: 00047
Certification File No.: 01162 Cert. Date: 02/08/2022 Cert. No.: 00039
Linearity File No.: 01163 Lin. Date: 02/08/2022 Lin. No.: 00038
Solution File No.: 01169 Soln. Date: 04/02/2022 Soln. No.: 00272
Sequential File No.: 01169 File Date: 04/02/2022

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUM S3-0225
Control Solution %: 0.100% Expires: 07/06/2022
Solution Control Lot: 20320 Bottle No.: 0741

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:04S		
Control 1 EC	0.100%	02:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:06S		
Control 2 EC	0.098%	02:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:07S		
Control 3 EC	0.098%	02:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CARDONE

First Name: ANTHONY

MI: D

Signature: _____



Badge No.: 4047

Date: 04/02/2022

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01161	Calib. Date: 02/08/2022
Certification File No.:	01162	Calib. No.: 00047
Linearity File No.:	01163	Cert. Date: 02/08/2022
Solution File No.:	01166	Cert. No.: 00039
Sequential File No.:	01166	Lin. Date: 02/08/2022
		Lin. No.: 00038
		Soln. Date: 03/06/2022
		Soln. No.: 00271
		File Date: 03/06/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0225
Solution Control Lot:	20320	Expires: 07/06/2022
		Bottle No.: 0575

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:08S		
Control 1 EC	0.098%	06:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:10S		
Control 2 EC	0.097%	06:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:11S		
Control 3 EC	0.099%	06:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LLOYD

First Name: MATTHEW

MI: T

Signature: _____



Badge No.: 4059

Date: 03/06/2022

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0053
Location:	FLORENCE TOWNSHIP P.D.	
Calibration File No.:	01143	Calib. Date: 09/08/2021
Certification File No.:	01144	Calib. No.: 00046
Linearity File No.:	01145	Cert. Date: 09/08/2021
Solution File No.:	01158	Cert. No.: 00038
Sequential File No.:	01158	Lin. Date: 09/08/2021
		Lin. No.: 00037
		Soln. Date: 01/16/2022
		Soln. No.: 00269
		File Date: 01/16/2022
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUM S3-0222
Solution Control Lot:	20320	Expires: 07/06/2022
		Bottle No.: 0330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:31S		
Control 1 EC	0.101%	18:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:33S		
Control 2 EC	0.099%	18:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:34S		
Control 3 EC	0.100%	18:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILK

First Name: JASON

MI: J

Signature: 

Badge No.: 4049

Date: 01/16/2022