

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. No.: 00013
Certification File No.:	00859	Cert. No.: 00011
Linearity File No.:	00860	Lin. No.: 00010
Solution File No.:	00921	Soln. No.: 00108
Sequential File No.:	00921	
	Calib. Date: 08/24/2010	
	Cert. Date: 08/24/2010	
	Lin. Date: 08/24/2010	
	Soln. Date: 12/22/2010	
	File Date: 12/22/2010	
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0681

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:25S		
Control 1 EC	0.098%	18:25S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:25S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:26S		
Control 2 EC	0.098%	18:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	18:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:27S		
Control 3 EC	0.098%	18:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	18:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BROWN

First Name: JOHN

MI: A

Signature: _____

Badge No.: 3201

Date: 12/22/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	00858	Calib. Date:	08/24/2010
Certification File No.:	00859	Cert. Date:	08/24/2010
Linearity File No.:	00860	Lin. Date:	08/24/2010
Solution File No.:	00917	Soln. Date:	12/15/2010
Sequential File No.:	00917	File Date:	12/15/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0699

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:07S		
Control 1 EC	0.101%	18:08S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:08S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:08S		
Control 2 EC	0.099%	18:09S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:09S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:10S		
Control 3 EC	0.100%	18:10S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:10S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 12/15/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. Date: 08/24/2010
Certification File No.:	00859	Calib. No.: 00013
Linearity File No.:	00860	Cert. Date: 08/24/2010
Solution File No.:	00903	Cert. No.: 00011
Sequential File No.:	00903	Lin. Date: 08/24/2010
		Lin. No.: 00010
		Soln. Date: 11/20/2010
		Soln. No.: 00106
		File Date: 11/20/2010


Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0680

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:37S		
Control 1 EC	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		
Control 2 EC	0.099%	10:38S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:38S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		
Control 3 EC	0.099%	10:40S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:40S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO	First Name: RONALD	MI: M
Signature: 		Badge No.: 3200 Date: 11/20/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. Date: 08/24/2010
Certification File No.:	00859	Cert. No.: 00013
Linearity File No.:	00860	Cert. Date: 08/24/2010
Solution File No.:	00892	Lin. No.: 00010
Sequential File No.:	00892	Lin. Date: 08/24/2010
		Soln. No.: 00105
		Soln. Date: 11/05/2010
		File Date: 11/05/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0683

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:58S		
Control 1 EC	0.100%	17:59S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:59S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:59S		
Control 2 EC	0.100%	18:00S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:00S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:01S		
Control 3 EC	0.100%	18:01S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:01S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____

Sgt. Robert Kelly

3204

Badge No.: 3204

Date: 11/05/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. Date: 08/24/2010
Certification File No.:	00859	Calib. No.: 00013
Linearity File No.:	00860	Cert. Date: 08/24/2010
Solution File No.:	00877	Cert. No.: 00011
Sequential File No.:	00877	Lin. Date: 08/24/2010
		Lin. No.: 00010
		Soln. Date: 10/09/2010
		Soln. No.: 00104
		File Date: 10/09/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0693

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:51D		
Control 1 EC	0.099%	13:51D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:51D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52D		
Control 2 EC	0.099%	13:53D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:53D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53D		
Control 3 EC	0.099%	13:54D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:54D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: Sgt. R Kelly

324

Badge No.: 3204

Date: 10/09/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00858	Calib. Date: 08/24/2010
Certification File No.:	00859	Calib. No.: 00013
Linearity File No.:	00860	Cert. Date: 08/24/2010
Solution File No.:	00868	Cert. No.: 00011
Sequential File No.:	00868	Lin. Date: 08/24/2010
		Lin. No.: 00010
		Soln. Date: 09/11/2010
		Soln. No.: 00103
		File Date: 09/11/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0684

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:50D		
Control 1 EC	0.100%	14:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51D		
Control 2 EC	0.100%	14:52D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:52D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:52D		
Control 3 EC	0.100%	14:53D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:53D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 09/11/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 00780 Calib. Date: 02/25/2010 Calib. No.: 00012
 Certification File No.: 00781 Cert. Date: 02/25/2010 Cert. No.: 00010
 Linearity File No.: 00782 Lin. Date: 02/25/2010 Lin. No.: 00009
 Solution File No.: 00849 Soln. Date: 07/27/2010 Soln. No.: 00100
 Sequential File No.: 00849 File Date: 07/27/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
 Control Solution %: 0.100% Expires: 02/02/2011
 Solution Control Lot: 09B063 Bottle No.: 0695

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:24D		
Control 1 EC	0.099%	16:25D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:26D		
Control 2 EC	0.100%	16:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:27D		
Control 3 EC	0.099%	16:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	16:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 07/27/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00780	Calib. Date: 02/25/2010
Certification File No.:	00781	Calib. No.: 00012
Linearity File No.:	00782	Cert. Date: 02/25/2010
Solution File No.:	00837	Cert. No.: 00010
Sequential File No.:	00837	Lin. Date: 02/25/2010
		Lin. No.: 00009
		Soln. Date: 07/01/2010
		Soln. No.: 00099
		File Date: 07/01/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0688

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:50D		
Control 1 EC	0.099%	16:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:52D		
Control 2 EC	0.099%	16:52D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.097%	16:52D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:53D		
Control 3 EC	0.098%	16:53D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	16:53D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

[Handwritten Signature] 63200

Badge No.: 3200

Date: 07/01/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00780	Calib. Date: 02/25/2010
Certification File No.:	00781	Calib. No.: 00012
Linearity File No.:	00782	Cert. Date: 02/25/2010
Solution File No.:	00826	Cert. No.: 00010
Sequential File No.:	00826	Lin. Date: 02/25/2010
		Lin. No.: 00009
		Soln. Date: 06/07/2010
		Soln. No.: 00098
		File Date: 06/07/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0690

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:14D		
Control 1 EC	0.100%	19:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:16D		
Control 2 EC	0.099%	19:16D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:16D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:17D		
Control 3 EC	0.100%	19:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 06/07/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00780	Calib. No.: 00012
Certification File No.:	00781	Cert. No.: 00010
Linearity File No.:	00782	Lin. No.: 00009
Solution File No.:	00809	Soln. No.: 00095
Sequential File No.:	00809	File Date: 05/03/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0687

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:39D		
Control 1 EC	0.100%	12:40D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:40D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40D		
Control 2 EC	0.100%	12:41D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42D		
Control 3 EC	0.100%	12:42D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:42D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature: _____

Badge No.: 3203

Date: 05/03/2010

Calibrating Unit

New Standard Solution Report


Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 00780 Calib. Date: 02/25/2010 Calib. No.: 00012
Certification File No.: 00781 Cert. Date: 02/25/2010 Cert. No.: 00010
Linearity File No.: 00782 Lin. Date: 02/25/2010 Lin. No.: 00009
Solution File No.: 00798 Soln. Date: 04/08/2010 Soln. No.: 00094
Sequential File No.: 00798 File Date: 04/08/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 02/02/2011
Solution Control Lot: 09B063 Bottle No.: 0682

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:02D		
Control 1 EC	0.100%	18:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:04D		
Control 2 EC	0.100%	18:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:05D		
Control 3 EC	0.099%	18:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	18:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

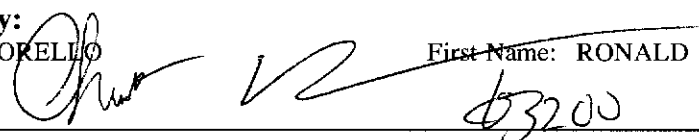Changed By:
Last Name: MORELLO First Name: RONALD MI: M
Signature:  Badge No.: 3200
Date: 04/08/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00780	Calib. Date: 02/25/2010
Certification File No.:	00781	Calib. No.: 00012
Linearity File No.:	00782	Cert. Date: 02/25/2010
Solution File No.:	00791	Cert. No.: 00010
Sequential File No.:	00791	Lin. Date: 02/25/2010
		Lin. No.: 00009
		Soln. Date: 03/13/2010
		Soln. No.: 00093
		File Date: 03/13/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0696

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:40S		
Control 1 EC	0.098%	09:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42S		
Control 2 EC	0.096%	09:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		
Control 3 EC	0.097%	09:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____

Handwritten signature
3202

Badge No.: 3202

Date: 03/13/2010

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	00698	Calib. Date:	08/25/2009
Certification File No.:	00699	Cert. Date:	08/25/2009
Linearity File No.:	00700	Lin. Date:	08/25/2009
Solution File No.:	00771	Soln. Date:	02/01/2010
Sequential File No.:	00771	File Date:	02/01/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	08F053	Expires:	06/09/2010
		Bottle No.:	0252

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:10S		
Control 1 EC	0.101%	16:11S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	16:11S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:12S		
Control 2 EC	0.101%	16:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:13S		
Control 3 EC	0.100%	16:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	16:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO	First Name: RONALD	MI: M
Signature: <u> 3200</u>		
	Badge No.:	3200
	Date:	02/01/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	00698	Calib. Date: 08/25/2009
Certification File No.:	00699	Cert. No.: 00011
Linearity File No.:	00700	Cert. Date: 08/25/2009
Solution File No.:	00762	Lin. Date: 08/25/2009
Sequential File No.:	00762	Lin. No.: 00008
		Soln. Date: 01/05/2010
		Soln. No.: 00089
		File Date: 01/05/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	08F053	Expires: 06/09/2010
		Bottle No.: 0251

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:32S		
Control 1 EC	0.101%	17:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	17:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:33S		
Control 2 EC	0.101%	17:34S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:34S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:35S		
Control 3 EC	0.101%	17:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	17:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:36S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 01/05/2010