

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01340	Calib. Date: 08/07/2012
Certification File No.:	01341	Calib. No.: 00025
Linearity File No.:	01342	Cert. Date: 08/07/2012
Solution File No.:	01470	Cert. No.: 00016
Sequential File No.:	01470	Lin. Date: 08/07/2012
		Lin. No.: 00015
		Soln. Date: 12/19/2012
		Soln. No.: 00164
		File Date: 12/19/2012

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0684

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:26S		
Control 1 EC	0.100%	13:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:27S		
Control 2 EC	0.099%	13:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:29S		
Control 3 EC	0.100%	13:29S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

 63200

Badge No.: 3200

Date: 12/19/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01340	Calib. Date:	08/07/2012
Certification File No.:	01341	Cert. Date:	08/07/2012
Linearity File No.:	01342	Lin. Date:	08/07/2012
Solution File No.:	01453	Soln. Date:	11/30/2012
Sequential File No.:	01453	File Date:	11/30/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	11H094	Expires:	08/17/2013
		Bottle No.:	0677

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:32S		
Control 1 EC	0.100%	04:33S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:34S		
Control 2 EC	0.099%	04:34S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:35S		
Control 3 EC	0.099%	04:36S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:36S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



#3204

Badge No.: 3204

Date: 11/30/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01340	Calib. Date: 08/07/2012
Certification File No.:	01341	Calib. No.: 00025
Linearity File No.:	01342	Cert. Date: 08/07/2012
Solution File No.:	01437	Cert. No.: 00016
Sequential File No.:	01437	Lin. Date: 08/07/2012
		Lin. No.: 00015
		Soln. Date: 11/15/2012
		Soln. No.: 00162
		File Date: 11/15/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0680

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:10S		
Control 1 EC	0.101%	18:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:11S		
Control 2 EC	0.099%	18:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:13S		
Control 3 EC	0.099%	18:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____

Steph MCBride

Badge No.: 3202

Date: 11/15/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 01340 Calib. Date: 08/07/2012 Calib. No.: 00025
 Certification File No.: 01341 Cert. Date: 08/07/2012 Cert. No.: 00016
 Linearity File No.: 01342 Lin. Date: 08/07/2012 Lin. No.: 00015
 Solution File No.: 01418 Soln. Date: 10/26/2012 Soln. No.: 00161
 Sequential File No.: 01418 File Date: 10/26/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
 Control Solution %: 0.100% Expires: 08/17/2013
 Solution Control Lot: 11H094 Bottle No.: 0679

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:09D		
Control 1 EC	0.101%	13:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:10D		
Control 2 EC	0.100%	13:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	13:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:12D		
Control 3 EC	0.100%	13:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:13D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/26/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01340	Calib. Date: 08/07/2012
Certification File No.:	01341	Calib. No.: 00025
Linearity File No.:	01342	Cert. Date: 08/07/2012
Solution File No.:	01396	Cert. No.: 00016
Sequential File No.:	01396	Lin. Date: 08/07/2012
		Lin. No.: 00015
		Soln. Date: 10/07/2012
		Soln. No.: 00160
		File Date: 10/07/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0678

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:04D		
Control 1 EC	0.099%	07:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:05D		
Control 2 EC	0.099%	07:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:06D		
Control 3 EC	0.099%	07:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

M1: J

Signature: _____

 # 3202

Badge No.: 3202

Date: 10/07/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01340 Calib. Date: 08/07/2012 Calib. No.: 00025
Certification File No.: 01341 Cert. Date: 08/07/2012 Cert. No.: 00016
Linearity File No.: 01342 Lin. Date: 08/07/2012 Lin. No.: 00015
Solution File No.: 01373 Soln. Date: 09/14/2012 Soln. No.: 00159
Sequential File No.: 01373 File Date: 09/14/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/17/2013
Solution Control Lot: 11H094 Bottle No.: 0676

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:40D		
Control 1 EC	0.103%	10:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	10:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 2 EC	0.102%	10:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		
Control 3 EC	0.101%	10:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 09/14/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01340	Calib. Date: 08/07/2012
Certification File No.:	01341	Calib. No.: 00025
Linearity File No.:	01342	Cert. Date: 08/07/2012
Solution File No.:	01356	Cert. No.: 00016
Sequential File No.:	01356	Lin. Date: 08/07/2012
		Lin. No.: 00015
		Soln. Date: 08/25/2012
		Soln. No.: 00158
		File Date: 08/25/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 08/17/2013
Solution Control Lot:	11H094		Bottle No.: 0685

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:57D		
Control 1 EC	0.099%	01:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	01:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:58D		
Control 2 EC	0.098%	01:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:00D		
Control 3 EC	0.098%	02:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



#3204

Badge No.: 3204

Date: 08/25/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01262	Calib. Date: 05/17/2012
Certification File No.:	01263	Calib. No.: 00019
Linearity File No.:	01264	Cert. Date: 05/17/2012
Solution File No.:	01326	Cert. No.: 00015
Sequential File No.:	01326	Lin. Date: 05/17/2012
		Lin. No.: 00014
		Soln. Date: 07/29/2012
		Soln. No.: 00150
		File Date: 07/29/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %:	0.100%		Expires: 08/17/2013
Solution Control Lot:	11H094		Bottle No.: 0690

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:32D		
Control 1 EC	0.098%	01:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:33D		
Control 2 EC	0.097%	01:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:34D		
Control 3 EC	0.097%	01:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	01:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____



Badge No.: 3202

Date: 07/29/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01262 Calib. Date: 05/17/2012 Calib. No.: 00019
Certification File No.: 01263 Cert. Date: 05/17/2012 Cert. No.: 00015
Linearity File No.: 01264 Lin. Date: 05/17/2012 Lin. No.: 00014
Solution File No.: 01313 Soln. Date: 07/18/2012 Soln. No.: 00149
Sequential File No.: 01313 File Date: 07/18/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 08/17/2013
Solution Control Lot: 11H094 Bottle No.: 0700

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:02D		
Control 1 EC	0.098%	10:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03D		
Control 2 EC	0.097%	10:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05D		
Control 3 EC	0.098%	10:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUJ2 - 030 (MPJ)

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P.

Signature:

M. P. Michael P. Gibson #6353

Badge No.: 6353

Date: 07/18/2012



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JEFFREY S. CHIESA
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 5/8/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12D101

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1204 to 0.1216 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 25, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Monica L. Tramontin
Monica L. Tramontin
Forensic Scientist III
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15th day of May, 2012.

Handwritten signature of Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



"An Internationally Accredited Agency"


New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael P. Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breath Test MKII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 14th DAY OF June

TWO THOUSAND AND Five

SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-3-07	OCPA	Wm Lora
2. 3-13-09	GCPA	Wm Lora
3. 2-3-11	OCPA	Wm Lora
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 08/03)


DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael Gibson
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breath Test Coordinator/Instructor
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 18th DAY OF June

TWO THOUSAND AND Eleven

SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 03/10)

DEPARTMENT OF
Law and Public Safety
This is to certify that

MICHAEL P. GIBSON
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE BREATHALYZER
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF October

TWO THOUSAND AND FOUR

SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 07/21 TO 07/25/2003


DATE	Refresher Course PLACE	INSTRUCTOR
1. 7-14-06	OCPA	Wm Lora
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 05/03)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Michael P. Gibson
North Wildwood City Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 25th DAY OF July

TWO THOUSAND AND 03

SUPERINTENDENT
NEW JERSEY STATE POLICE


ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 06/03)



CERTIFICATE

This is to certify that

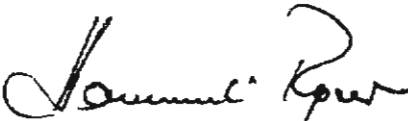
Michael P. Gibson #6353

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

Operator Trainer and Maintenance Technician

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 18, 2011



Instructor: Hansueli Ryser

Dräger



CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lieutenant Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF CRIMINAL JUSTICE
PO BOX 085
TRENTON, NJ 08625-0085
TELEPHONE: (609) 984-6500

PAULA T. DOW
Attorney General

STEPHEN J. TAYLOR
Director

June 10, 2011

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification - Trooper Michael Gibson #6353

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Trooper Michael Gibson #6353, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Paula Dow
Attorney General

- c. Trooper Michael Gibson #6353, Alcohol/Drug Test Unit, Division of State Police
Lt. Craig Potter, Unit Head, Alcohol/Drug Test Unit, Division of State Police



Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01262 Calib. Date: 05/17/2012 Calib. No.: 00019
Certification File No.: 01263 Cert. Date: 05/17/2012 Cert. No.: 00015
Linearity File No.: 01264 Lin. Date: 05/17/2012 Lin. No.: 00014
Solution File No.: 01306 Soln. Date: 07/12/2012 Soln. No.: 00148
Sequential File No.: 01306 File Date: 07/12/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 08/17/2013
Solution Control Lot: 11H094 Bottle No.: 0689

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:30D		
Control 1 EC	0.098%	10:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	10:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31D		
Control 2 EC	0.097%	10:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33D		
Control 3 EC	0.098%	10:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

M1: M

Signature:  3200

Badge No.: 3200

Date: 07/12/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01262	Calib. Date: 05/17/2012
Certification File No.:	01263	Calib. No.: 00019
Linearity File No.:	01264	Cert. Date: 05/17/2012
Solution File No.:	01305	Cert. No.: 00015
Sequential File No.:	01305	Lin. Date: 05/17/2012
		Lin. No.: 00014
		Soln. Date: 07/10/2012
		Soln. No.: 00147
		File Date: 07/10/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %:	0.100%		Expires: 08/17/2013
Solution Control Lot:	11H094		Bottle No.: 0695

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:29D		
Control 1 EC	0.097%	07:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:30D		
Control 2 EC	0.097%	07:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	07:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:31D		
Control 3 EC	0.097%	07:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	07:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____

A 3202

Badge No.: 3202

Date: 07/10/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 01262 Calib. Date: 05/17/2012 Calib. No.: 00019
 Certification File No.: 01263 Cert. Date: 05/17/2012 Cert. No.: 00015
 Linearity File No.: 01264 Lin. Date: 05/17/2012 Lin. No.: 00014
 Solution File No.: 01296 Soln. Date: 06/28/2012 Soln. No.: 00146
 Sequential File No.: 01296 File Date: 06/28/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
 Control Solution %: 0.100% Expires: 08/17/2013
 Solution Control Lot: 11H094 Bottle No.: 0699

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:19D		
Control 1 EC	0.098%	03:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	03:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:20D		
Control 2 EC	0.097%	03:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:22D		
Control 3 EC	0.097%	03:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	03:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.



Changed By:

Last Name: KELLY

First Name: ROBERT

M1: J

Signature: _____

Badge No.: 3204

Date: 06/28/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01262	Calib. Date: 05/17/2012
Certification File No.:	01263	Cert. No.: 00019
Linearity File No.:	01264	Cert. Date: 05/17/2012
Solution File No.:	01289	Lin. No.: 00014
Sequential File No.:	01289	Soln. Date: 06/16/2012
		Soln. No.: 00145
		File Date: 06/16/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0681

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:20D		
Control 1 EC	0.097%	05:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	05:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21D		
Control 2 EC	0.097%	05:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	05:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:23D		
Control 3 EC	0.097%	05:24D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.096%	05:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____



Badge No.: 3202

Date: 06/16/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01262	Calib. Date: 05/17/2012
Certification File No.:	01263	Calib. No.: 00019
Linearity File No.:	01264	Cert. Date: 05/17/2012
Solution File No.:	01280	Cert. No.: 00015
Sequential File No.:	01280	Lin. Date: 05/17/2012
		Lin. No.: 00014
		Soln. Date: 06/02/2012
		Soln. No.: 00144
		File Date: 06/02/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %:	0.100%		Expires: 08/17/2013
Solution Control Lot:	11H094		Bottle No.: 0691

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:03D		
Control 1 EC	0.098%	19:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	19:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:05D		
Control 2 EC	0.097%	19:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:06D		
Control 3 EC	0.098%	19:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



3204

Badge No.: 3204

Date: 06/02/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01136	Calib. Date: 11/23/2011
Certification File No.:	01137	Calib. No.: 00018
Linearity File No.:	01138	Cert. Date: 11/23/2011
Solution File No.:	01261	Cert. No.: 00014
Sequential File No.:	01261	Lin. Date: 11/23/2011
		Lin. No.: 00013
		Soln. Date: 05/13/2012
		Soln. No.: 00142
		File Date: 05/13/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0683

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:08D		
Control 1 EC	0.100%	05:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:09D		
Control 2 EC	0.100%	05:10D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:11D		
Control 3 EC	0.100%	05:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



3004

Badge No.: 3204

Date: 05/13/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01136 Calib. Date: 11/23/2011 Calib. No.: 00018
Certification File No.: 01137 Cert. Date: 11/23/2011 Cert. No.: 00014
Linearity File No.: 01138 Lin. Date: 11/23/2011 Lin. No.: 00013
Solution File No.: 01241 Soln. Date: 04/19/2012 Soln. No.: 00141
Sequential File No.: 01241 File Date: 04/19/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/17/2013
Solution Control Lot: 11H094 Bottle No.: 0696

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:25D		
Control 1 EC	0.100%	10:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26D		
Control 2 EC	0.099%	10:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:28D		
Control 3 EC	0.099%	10:28D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

 3200

Badge No.: 3200

Date: 04/19/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01136 Calib. Date: 11/23/2011 Calib. No.: 00018
Certification File No.: 01137 Cert. Date: 11/23/2011 Cert. No.: 00014
Linearity File No.: 01138 Lin. Date: 11/23/2011 Lin. No.: 00013
Solution File No.: 01228 Soln. Date: 03/24/2012 Soln. No.: 00140
Sequential File No.: 01228 File Date: 03/24/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/17/2013
Solution Control Lot: 11H094 Bottle No.: 0682

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:29S		
Control 1 EC	0.100%	10:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31S		
Control 2 EC	0.100%	10:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32S		
Control 3 EC	0.100%	10:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 03/24/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01136	Calib. Date: 11/23/2011
Certification File No.:	01137	Calib. No.: 00018
Linearity File No.:	01138	Cert. Date: 11/23/2011
Solution File No.:	01213	Cert. No.: 00014
Sequential File No.:	01213	Lin. Date: 11/23/2011
		Lin. No.: 00013
		Soln. Date: 03/06/2012
		Soln. No.: 00139
		File Date: 03/06/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 08/17/2013
Solution Control Lot:	11H094		Bottle No.: 0686

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:30S		
Control 1 EC	0.099%	02:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:32S		
Control 2 EC	0.098%	02:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:33S		
Control 3 EC	0.099%	02:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____

 # 3202

Badge No.: 3202

Date: 03/06/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01136	Calib. Date:	11/23/2011
Certification File No.:	01137	Cert. No.:	00018
Linearity File No.:	01138	Cert. Date:	11/23/2011
Solution File No.:	01197	Lin. No.:	00013
Sequential File No.:	01197	Soln. Date:	02/21/2012
		Soln. No.:	00138
		File Date:	02/21/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	11H094	Expires:	08/17/2013
		Bottle No.:	0687

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:40S		
Control 1 EC	0.101%	12:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41S		
Control 2 EC	0.100%	12:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42S		
Control 3 EC	0.100%	12:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

[Handwritten Signature] 63200

Badge No.: 3200

Date: 02/21/2012

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01136	Calib. Date:	11/23/2011
Certification File No.:	01137	Cert. Date:	11/23/2011
Linearity File No.:	01138	Lin. Date:	11/23/2011
Solution File No.:	01184	Soln. Date:	02/03/2012
Sequential File No.:	01184	File Date:	02/03/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	11H094	Expires:	08/17/2013
		Bottle No.:	0698

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:38S		
Control 1 EC	0.100%	04:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:40S		
Control 2 EC	0.099%	04:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:41S		
Control 3 EC	0.099%	04:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE	First Name: STEPHEN	MI: J
Signature: 	# 3202	Badge No.: 3202
		Date: 02/03/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01136	Calib. Date:	11/23/2011
Certification File No.:	01137	Cert. Date:	11/23/2011
Linearity File No.:	01138	Lin. Date:	11/23/2011
Solution File No.:	01170	Soln. Date:	01/13/2012
Sequential File No.:	01170	File Date:	01/13/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	11H094	Expires:	08/17/2013
		Bottle No.:	0688

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:48S		
Control 1 EC	0.099%	16:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:49S		
Control 2 EC	0.098%	16:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	16:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:51S		
Control 3 EC	0.098%	16:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	16:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:52S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

 63200

Badge No.: 3200

Date: 01/13/2012