

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01957 Calib. Date: 10/20/2014 Calib. No.: 00030
Certification File No.: 01958 Cert. Date: 10/20/2014 Cert. No.: 00021
Linearity File No.: 01959 Lin. Date: 10/20/2014 Lin. No.: 00020
Solution File No.: 01999 Soln. Date: 12/19/2014 Soln. No.: 00217
Sequential File No.: 01999 File Date: 12/19/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
Control Solution %: 0.100% Expires: 04/29/2016
Solution Control Lot: 14D129 Bottle No.: 1186

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:18S		
Control 1 EC	0.100%	11:19S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20S		
Control 2 EC	0.099%	11:20S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21S		
Control 3 EC	0.099%	11:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 12/19/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01957	Calib. Date: 10/20/2014
Certification File No.:	01958	Calib. No.: 00030
Linearity File No.:	01959	Cert. Date: 10/20/2014
Solution File No.:	01998	Cert. No.: 00021
Sequential File No.:	01998	Lin. Date: 10/20/2014
		Lin. No.: 00020
		Soln. Date: 12/19/2014
		Soln. No.: 00216
		File Date: 12/19/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %: 0.100%		Expires: 04/29/2016
Solution Control Lot: 14D129		Bottle No.: 1181

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:27S		
Control 1 EC	-.---%	09:27S	21.1°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	09:27S	21.1°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 12/19/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01957	Calib. Date: 10/20/2014
Certification File No.:	01958	Calib. No.: 00030
Linearity File No.:	01959	Cert. Date: 10/20/2014
Solution File No.:	01985	Cert. No.: 00021
Sequential File No.:	01985	Lin. Date: 10/20/2014
		Lin. No.: 00020
		Soln. Date: 12/05/2014
		Soln. No.: 00215
		File Date: 12/05/2014

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %:	0.100%		Expires: 04/29/2016
Solution Control Lot:	14D129		Bottle No.: 1179

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:02S		
Control 1 EC	0.100%	10:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03S		
Control 2 EC	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05S		
Control 3 EC	0.100%	10:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 12/05/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT		
Calibration File No.:	01957	Calib. Date:	10/20/2014
Certification File No.:	01958	Calib. No.:	00030
Linearity File No.:	01959	Cert. Date:	10/20/2014
Solution File No.:	01971	Lin. No.:	00020
Sequential File No.:	01971	Soln. Date:	11/13/2014
		Soln. No.:	00214
		File Date:	11/13/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	1180

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:21S		
Control 1 EC	0.101%	13:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22S		
Control 2 EC	0.098%	13:23S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:24S		
Control 3 EC	0.099%	13:24S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:24S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:25S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

M1: M

Signature: 

Badge No.: 3200

Date: 11/13/2014

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
Solution File No.: 01949 Soln. Date: 10/11/2014 Soln. No.: 00212
Sequential File No.: 01949 File Date: 10/11/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 12/26/2014
Solution Control Lot: 12L109 Bottle No.: 0412

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:13D		
Control 1 EC	0.098%	14:14D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	14:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:14D		
Control 2 EC	0.097%	14:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:16D		
Control 3 EC	0.097%	14:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:17D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/11/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Cert. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01948	Lin. No.: 00019
Sequential File No.:	01948	Lin. Date: 05/09/2014
		Soln. No.: 00211
		Soln. Date: 10/11/2014
		File Date: 10/11/2014

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	12L109	Expires: 12/26/2014
		Bottle No.: 0403

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:23D		
Control 1 EC	0.098%	12:23D	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	----%	12:23D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	----%	12:24D		
Control 2 EC	----%	--:--	N/A	
Control 2 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		
Control 3 EC	----%	--:--	N/A	
Control 3 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

M1: M

Signature: _____



Badge No.: 3200

Date: 10/11/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01942	Cert. No.: 00020
Sequential File No.:	01942	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 10/01/2014
		Soln. No.: 00210
		File Date: 10/01/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %: 0.100%		Expires: 12/26/2014
Solution Control Lot: 12L109		Bottle No.: 0424

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:19D		
Control 1 EC	0.098%	10:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:21D		
Control 2 EC	0.097%	10:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		
Control 3 EC	0.098%	10:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.095%	10:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 10/01/2014

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
 Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
 Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
 Solution File No.: 01941 Soln. Date: 10/01/2014 Soln. No.: 00209
 Sequential File No.: 01941 File Date: 10/01/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
 Control Solution %: 0.100% Expires: 12/26/2014
 Solution Control Lot: 12L109 Bottle No.: 0421

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:15D		
Control 1 EC	----%	09:16D	N/A	TEST RESET
Control 1 IR	----%	09:16D	N/A	TEST RESET
Ambient Air Blank	----%	---:---		
Control 2 EC	----%	---:---	N/A	
Control 2 IR	----%	---:---	N/A	
Ambient Air Blank	----%	---:---		
Control 3 EC	----%	---:---	N/A	
Control 3 IR	----%	---:---	N/A	
Ambient Air Blank	----%	---:---		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 10/01/2014

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
Solution File No.: 01928 Soln. Date: 09/19/2014 Soln. No.: 00208
Sequential File No.: 01928 File Date: 09/19/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 12/26/2014
Solution Control Lot: 12L109 Bottle No.: 0411

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:04D		
Control 1 EC	0.099%	10:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05D		
Control 2 EC	0.097%	10:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07D		
Control 3 EC	0.097%	10:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08D		

All tests within acceptable tolerance.

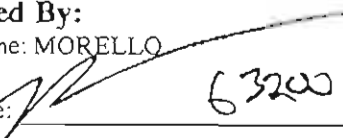
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 09/19/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01919	Cert. No.: 00020
Sequential File No.:	01919	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 09/06/2014
		Soln. No.: 00207
		File Date: 09/06/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	12/26/2014
Solution Control Lot:	12L109			Bottle No.:	0413

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:25D		
Control 1 EC	0.098%	23:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:27D		
Control 2 EC	0.097%	23:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	23:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:28D		
Control 3 EC	0.097%	23:29D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	23:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:29D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 09/06/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01906	Cert. No.: 00020
Sequential File No.:	01906	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 08/21/2014
		Soln. No.: 00206
		File Date: 08/21/2014

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	12L109	Expires: 12/26/2014
		Bottle No.: 0406

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:42D		
Control 1 EC	0.099%	16:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:43D		
Control 2 EC	0.098%	16:44D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	16:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44D		
Control 3 EC	0.098%	16:45D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:46D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 08/21/2014

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
Solution File No.: 01894 Soln. Date: 08/03/2014 Soln. No.: 00205
Sequential File No.: 01894 File Date: 08/03/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 12/26/2014
Solution Control Lot: 12L109 Bottle No.: 0422

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:38D		
Control 1 EC	0.099%	01:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	01:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:40D		
Control 2 EC	0.097%	01:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	01:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:41D		
Control 3 EC	0.097%	01:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	01:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:42D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 08/03/2014

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
Solution File No.: 01887 Soln. Date: 07/20/2014 Soln. No.: 00204
Sequential File No.: 01887 File Date: 07/20/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 12/26/2014
Solution Control Lot: 12L109 Bottle No.: 0417

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:44D		
Control 1 EC	0.099%	10:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45D		
Control 2 EC	0.099%	10:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		
Control 3 EC	0.099%	10:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



6320

Badge No.: 3200

Date: 07/20/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01871	Cert. No.: 00020
Sequential File No.:	01871	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 06/21/2014
		Soln. No.: 00202
		File Date: 06/21/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %: 0.100%		Expires: 12/26/2014
Solution Control Lot: 12L109		Bottle No.: 0408

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:13D		
Control 1 EC	0.097%	11:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		
Control 2 EC	0.097%	11:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	11:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16D		
Control 3 EC	0.097%	11:17D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	11:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 06/21/2014

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 01835 Calib. Date: 05/09/2014 Calib. No.: 00029
Certification File No.: 01836 Cert. Date: 05/09/2014 Cert. No.: 00020
Linearity File No.: 01837 Lin. Date: 05/09/2014 Lin. No.: 00019
Solution File No.: 01865 Soln. Date: 06/09/2014 Soln. No.: 00201
Sequential File No.: 01865 File Date: 06/09/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 12/26/2014
Solution Control Lot: 12L109 Bottle No.: 0407

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:58D		
Control 1 EC	0.097%	13:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59D		
Control 2 EC	0.097%	14:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00D		
Control 3 EC	0.097%	14:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	14:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:02D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: 

#3204

Badge No.: 3204

Date: 06/09/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01855	Cert. No.: 00020
Sequential File No.:	01855	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 05/23/2014
		Soln. No.: 00200
		File Date: 05/23/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDIJK S3-0133
Control Solution %: 0.100%		Expires: 12/26/2014
Solution Control Lot: 12L109		Bottle No.: 0404

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:29D		
Control 1 EC	0.098%	18:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:31D		
Control 2 EC	0.098%	18:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:32D		
Control 3 EC	0.097%	18:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	18:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 05/23/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01835	Calib. Date: 05/09/2014
Certification File No.:	01836	Calib. No.: 00029
Linearity File No.:	01837	Cert. Date: 05/09/2014
Solution File No.:	01850	Cert. No.: 00020
Sequential File No.:	01850	Lin. Date: 05/09/2014
		Lin. No.: 00019
		Soln. Date: 05/18/2014
		Soln. No.: 00199
		File Date: 05/18/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	12L109	Expires: 12/26/2014
		Bottle No.: 0423

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:18D		
Control 1 EC	0.097%	06:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	06:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:19D		
Control 2 EC	0.097%	06:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	06:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:20D		
Control 3 EC	0.097%	06:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

M1: J

Signature: _____



3204

Badge No.: 3204

Date: 05/18/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01835	Calib. Date:	05/09/2014
Certification File No.:	01836	Cert. Date:	05/09/2014
Linearity File No.:	01837	Lin. Date:	05/09/2014
Solution File No.:	01849	Soln. Date:	05/18/2014
Sequential File No.:	01849	File Date:	05/18/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	12/26/2014
Solution Control Lot:	12L109			Bottle No.:	0409

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:01D		
Control 1 EC	-.---%	05:02D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	05:02D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3204

Date: 05/18/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcoest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cert. Date:	12/03/2013
Linearity File No.:	01731	Lin. Date:	12/03/2013
Solution File No.:	01834	Soln. Date:	05/08/2014
Sequential File No.:	01834	File Date:	05/08/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DOUL S3-0163
Control Solution %:	0.100%			Expires:	12/26/2014
Solution Control Lot:	12L109			Bottle No.:	0416

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:03D		
Control 1 EC	0.100%	10:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05D		
Control 2 EC	0.099%	10:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		
Control 3 EC	0.099%	10:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcoest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 05/08/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location	STRATFORD POLICE DEPT.		
Calibration File No.	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cert. Date:	12/03/2013
Linearity File No.	01731	Lin. Date:	12/03/2013
Solution File No.:	01817	Soln. Date:	04/19/2014
Sequential File No.:	01817	File Date:	04/19/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0410

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	of Error(s)
Ambient Air Blank	0.000%	09:37D		
Control 1 EC	0.101%	09:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38D		
Control 2 EC	0.099%	09:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40D		
Control 3 EC	0.100%	09:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: ~

Signature: _____



Badge No. 3200

Date: 04/19/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cert. Date:	12/03/2013
Linearity File No.:	01731	Lin. Date:	12/03/2013
Solution File No.:	01802	Soln. Date:	04/01/2014
Sequential File No.:	01802	File Date:	04/01/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0425

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:34S		
Control 1 EC	0.100%	09:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35S		
Control 2 EC	0.099%	09:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:37S		
Control 3 EC	0.100%	09:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 04/01/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cert. Date:	12/03/2013
Linearity File No.:	01731	Lin. Date:	12/03/2013
Solution File No.:	01784	Soln. Date:	03/04/2014
Sequential File No.:	01784	File Date:	03/04/2014
Calibrating Unit:	WET	Model No.:	CU-J4
Control Solution %:	0.100%	Serial No.:	DDJL S3-0183
Solution Control Loc:	12L109	Expires:	12/26/2014
		Bottle No.:	0418

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:29S		
Control 1 EC	0.100%	12:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30S		
Control 2 EC	0.099%	12:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32S		
Control 3 EC	0.100%	12:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NISP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

M. M.

Signature: _____

Badge No.: 3200

Date: 03/04/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT		
Calibration File No.:	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cert. Date:	12/03/2013
Linearity File No.:	01731	Lin. Date:	12/03/2013
Solution File No.:	01770	Soln. Date:	02/10/2014
Sequential File No.:	01770	File Date:	02/10/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDU1-S3-0163
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0414

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:46S		
Control 1 EC	0.100%	14:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:48S		
Control 2 EC	0.099%	14:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:49S		
Control 3 EC	0.099%	14:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist

Changed By:

Last Name: MORENO

First Name: RONALD

MLM

Signature: _____

Badge No. 3200

Date: 02/10/2014


Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01729	Calib. Date:	12/03/2013
Certification File No.:	01730	Cen. Date:	12/03/2013
Linearity File No.:	01731	Lin. Date:	12/03/2013
Solution File No.:	01758	Soln. Date:	01/22/2014
Sequential File No.:	01758	File Date:	01/22/2014
Calibrating Unit:	WET	Model No.:	CU-J4
Control Solution %:	0.100%	Serial No.:	DDUL S3-016J
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0419

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:58S		
Control 1 EC	0.099%	11:58S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S		
Control 2 EC	0.097%	12:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	12:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01S		
Control 3 EC	0.099%	12:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:			
Last Name: MORELLO	First Name: RONALD		MJ: M
Signature: 		Badge No.: 3200	
		Date: 01/22/2014	

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01729	Calib. Date: 12/03/2013
Certification File No.:	01730	Calib. No.: 00028
Linearity File No.:	01731	Cert. Date: 12/03/2013
Solution File No.:	01749	Cert. No.: 00019
Sequential File No.:	01749	Lin. Date: 12/03/2013
		Lin. No.: 00018
		Soln. Date: 01/03/2014
		Soln. No.: 00190
		File Date: 01/03/2014

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %: 0.100%		Expires: 12/26/2014
Solution Control Lot: 12L109		Bottle No.: 0415

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:55S		
Control 1 EC	0.099%	12:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:56S		
Control 2 EC	0.099%	12:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:58S		
Control 3 EC	0.099%	12:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:59S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  3200

Badge No.: 3200

Date: 01/03/2014