

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02406	Cert. No.: 00025
Sequential File No.:	02406	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 12/31/2016
		Soln. No.: 00259
		File Date: 12/31/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 08/04/2017
Solution Control Lot:	15H140		Bottle No.: 0172

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:41S		
Control 1 EC	0.100%	11:42S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:43S		
Control 2 EC	0.098%	11:44S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:45S		
Control 3 EC	0.099%	11:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:46S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  _____

Badge No.: 3200

Date: 12/31/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02329	Calib. Date:	07/06/2016
Certification File No.:	02330	Cert. No.:	00034
Linearity File No.:	02331	Lin. Date:	07/06/2016
Solution File No.:	02403	Cert. No.:	00025
Sequential File No.:	02403	Lin. No.:	00024
		Soln. Date:	12/23/2016
		Soln. No.:	00258
		File Date:	12/23/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	0166

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:11S		
Control 1 EC	0.100%	10:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:12S		
Control 2 EC	0.099%	10:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14S		
Control 3 EC	0.100%	10:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

[Handwritten Signature]
63200

Badge No.: 3200

Date: 12/23/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02400	Cert. No.: 00025
Sequential File No.:	02400	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 12/16/2016
		Soln. No.: 00257
		File Date: 12/16/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0161

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:14S		
Control 1 EC	0.104%	15:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:15S		
Control 2 EC	0.101%	15:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 3 EC	0.101%	15:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	15:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 12/16/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02394	Cert. No.: 00025
Sequential File No.:	02394	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 12/09/2016
		Soln. No.: 00256
		File Date: 12/09/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 08/04/2017
Solution Control Lot:	15H140		Bottle No.: 0158

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:08S		
Control 1 EC	0.101%	10:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09S		
Control 2 EC	0.099%	10:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:11S		
Control 3 EC	0.101%	10:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

Badge No.: 3200

Date: 12/09/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02329	Calib. Date:	07/06/2016
Certification File No.:	02330	Cert. Date:	07/06/2016
Linearity File No.:	02331	Lin. Date:	07/06/2016
Solution File No.:	02390	Soln. Date:	11/28/2016
Sequential File No.:	02390	File Date:	11/28/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	08/04/2017
Solution Control Lot:	15H140			Bottle No.:	0151

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:57S		
Control 1 EC	0.101%	09:58S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:58S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58S		
Control 2 EC	0.099%	09:59S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:59S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00S		
Control 3 EC	0.101%	10:01S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

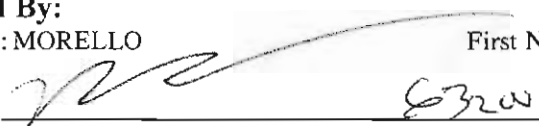
Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____



Badge No.: 3200

Date: 11/28/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02329	Calib. Date:	07/06/2016
Certification File No.:	02330	Cert. Date:	07/06/2016
Linearity File No.:	02331	Lin. Date:	07/06/2016
Solution File No.:	02388	Soln. Date:	11/27/2016
Sequential File No.:	02388	File Date:	11/27/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	0173

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:33S		
Control 1 EC	0.101%	10:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35S		
Control 2 EC	0.100%	10:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 3 EC	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

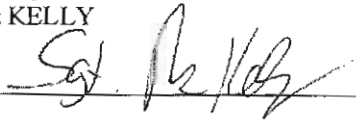
Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3204

Date: 11/27/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02379	Cert. No.: 00025
Sequential File No.:	02379	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 11/06/2016
		Soln. No.: 00253
		File Date: 11/06/2016

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0167

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:08S		
Control 1 EC	0.102%	09:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:10S		
Control 2 EC	0.101%	09:11S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11S		
Control 3 EC	0.101%	09:12S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  6320

Badge No.: 3200

Date: 11/06/2016

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: STRATFORD POLICE DEPT. Serial No.: ARNK-0039
Calibration File No.: 02329 Calib. Date: 07/06/2016 Calib. No.: 00034
Certification File No.: 02330 Cert. Date: 07/06/2016 Cert. No.: 00025
Linearity File No.: 02331 Lin. Date: 07/06/2016 Lin. No.: 00024
Solution File No.: 02369 Soln. Date: 10/27/2016 Soln. No.: 00252
Sequential File No.: 02369 File Date: 10/27/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0162

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:01D		
Control 1 EC	0.102%	11:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	11:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03D		
Control 2 EC	0.100%	11:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		
Control 3 EC	0.100%	11:05D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/27/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 02329 Calib. Date: 07/06/2016 Calib. No.: 00034
Certification File No.: 02330 Cert. Date: 07/06/2016 Cert. No.: 00025
Linearity File No.: 02331 Lin. Date: 07/06/2016 Lin. No.: 00024
Solution File No.: 02360 Soln. Date: 10/05/2016 Soln. No.: 00251
Sequential File No.: 02360 File Date: 10/05/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0168

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:10D		
Control 1 EC	0.100%	17:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:12D		
Control 2 EC	0.099%	17:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:13D		
Control 3 EC	0.099%	17:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	17:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:15D		

All tests within acceptable tolerance.

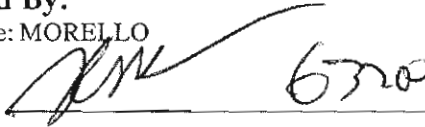
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 10/05/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02355	Cert. No.: 00025
Sequential File No.:	02355	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 09/12/2016
		Soln. No.: 00250
		File Date: 09/12/2016

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 08/04/2017
Solution Control Lot:	15H140		Bottle No.: 0152

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:43D		
Control 1 EC	0.102%	10:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44D		
Control 2 EC	0.100%	10:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45D		
Control 3 EC	0.100%	10:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 09/12/2016

Signature:  63200

Badge No.: 3200

Date: 09/12/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
Location: STRATFORD POLICE DEPT.
Calibration File No.: 02329 Calib. Date: 07/06/2016 Calib. No.: 00034
Certification File No.: 02330 Cert. Date: 07/06/2016 Cert. No.: 00025
Linearity File No.: 02331 Lin. Date: 07/06/2016 Lin. No.: 00024
Solution File No.: 02346 Soln. Date: 08/21/2016 Soln. No.: 00249
Sequential File No.: 02346 File Date: 08/21/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133
Control Solution %: 0.100% Expires: 08/04/2017
Solution Control Lot: 15H140 Bottle No.: 0157

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:02D		
Control 1 EC	0.102%	12:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04D		
Control 2 EC	0.101%	12:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05D		
Control 3 EC	0.101%	12:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

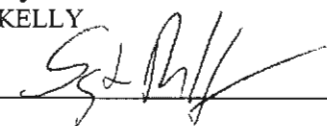
Changed By:

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: _____



Badge No.: 3204

Date: 08/21/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02329	Calib. Date: 07/06/2016
Certification File No.:	02330	Calib. No.: 00034
Linearity File No.:	02331	Cert. Date: 07/06/2016
Solution File No.:	02337	Cert. No.: 00025
Sequential File No.:	02337	Lin. Date: 07/06/2016
		Lin. No.: 00024
		Soln. Date: 07/28/2016
		Soln. No.: 00248
		File Date: 07/28/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0153

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:24D		
Control 1 EC	0.102%	09:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		
Control 2 EC	0.100%	09:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27D		
Control 3 EC	0.100%	09:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: _____



3202

Badge No.: 3202

Date: 07/28/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02249	Calib. Date: 02/11/2016
Certification File No.:	02250	Calib. No.: 00033
Linearity File No.:	02251	Cert. Date: 02/11/2016
Solution File No.:	02323	Cert. No.: 00024
Sequential File No.:	02323	Lin. Date: 02/11/2016
		Lin. No.: 00023
		Soln. Date: 06/18/2016
		Soln. No.: 00246
		File Date: 06/18/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0163

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:29D		
Control 1 EC	0.104%	10:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	10:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:30D		
Control 2 EC	0.100%	10:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32D		
Control 3 EC	0.101%	10:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	10:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:


Last Name: MORELLO

First Name: RONALD


MI: M

Signature:  # 3200

Badge No.: 3200
Date: 06/18/2016

Signature:  # 3200

Badge No.: 3200
Date: 06/18/2016

Signature:  # 3200

Badge No.: 3200
Date: 06/18/2016

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0039
 Location: STRATFORD POLICE DEPT.
 Calibration File No.: 02249 Calib. Date: 02/11/2016 Calib. No.: 00033
 Certification File No.: 02250 Cert. Date: 02/11/2016 Cert. No.: 00024
 Linearity File No.: 02251 Lin. Date: 02/11/2016 Lin. No.: 00023
 Solution File No.: 02312 Soln. Date: 05/25/2016 Soln. No.: 00245
 Sequential File No.: 02312 File Date: 05/25/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163
 Control Solution %: 0.100% Expires: 08/04/2017
 Solution Control Lot: 15H140 Bottle No.: 0175


Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:15D		
Control 1 EC	0.104%	13:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	13:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		
Control 2 EC	0.102%	13:17D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.104%	13:17D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18D		
Control 3 EC	0.104%	13:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	13:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO First Name: RONALD MI: M

Signature:  Badge No.: 3200
Date: 05/25/2016

Signature:  Badge No.: 3200
Date: 05/25/2016

Signature:  Badge No.: 3200
Date: 05/25/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02249	Calib. Date:	02/11/2016
Certification File No.:	02250	Cert. No.:	00033
Linearity File No.:	02251	Lin. Date:	02/11/2016
Solution File No.:	02295	Lin. No.:	00024
Sequential File No.:	02295	Soln. Date:	04/29/2016
		Soln. No.:	00244
		File Date:	04/29/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	0164

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:31D		
Control 1 EC	0.104%	10:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32D		
Control 2 EC	0.102%	10:33D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:33D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33D		
Control 3 EC	0.102%	10:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	10:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

63800

Badge No.: 3200

Date: 04/29/2016

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No:	02249	Calib. Date: 02/11/2016
Certification File No.:	02250	Cert. No.: 00024
Library File No.:	02251	Lin. No.: 00024
Solution File No.:	02279	Soln. No.: 00243
Sequential File No.:	02279	File Date: 04/05/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL 53-0163
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 0154

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:49D		
Control 1 EC	0.104%	10:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	10:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:51D		
Control 2 EC	0.101%	10:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	10:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52D		
Control 3 EC	0.102%	10:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	10:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO	First Name: RONALD	MI: M
Signature: 	Badge No: 3200	Date: 04/05/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcores 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02249	Calib. Date:	02/11/2016
Certification File No.:	02250	Cert. Date:	02/11/2016
Linearity File No.:	02251	Lin. Date:	02/11/2016
Solution File No.:	02269	Soln. Date:	03/11/2016
Sequential File No.:	02269	File Date:	03/11/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL 53-0163
Solution Control Lot:	14D129	Expires:	04/29/2016
		Bottle No.:	1190

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:31S		
Control 1 EC	0.103%	17:31S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.103%	17:31S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:32S		
Control 2 EC	0.101%	17:33S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.104%	17:33S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:34S		
Control 3 EC	0.103%	17:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	17:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:35S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcores 7110 operator training and procedures established by the (NISP) Chief Forensic Scientist.

Changed By:


Last Name: MORELLO

First Name: RONALD


MI: M

Signature:  3200

Badge No.: 3200
Date: 03/11/2016

Signature:  3200

Badge No.: 3200
Date: 03/11/2016

Signature:  3200

Badge No.: 3200
Date: 03/11/2016

Calibrating Unit New Standard Solution Report

Equipment	Alcoatest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02155	Calib. Date:	09/01/2015
Certification File No.:	02156	Cert. Date:	09/01/2015
Linearity File No.:	02157	Lin. Date:	09/01/2015
Solution File No.:	02241	Soln. Date:	01/22/2016
Sequential File No.:	02241	File Date:	01/22/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	08/04/2017
Solution Control Lot:	15H140			Bottle No.:	0159

Function	Result %BAC	Time MM:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:44S		
Control 1 EC	0.101%	15:44S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:45S		
Control 2 EC	0.101%	15:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:47S		
Control 3 EC	0.101%	15:48S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcoatest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: _____

 63200

Badge No.: 3200

Date: 01/22/2016

Signature: _____

 63200

Badge No.: 3200

Date: 01/22/2016

Signature: _____

 63200

Badge No.: 3200

Date: 01/22/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT	Calib. No.:	00032
Calibration File No.:	02155	Calib. Date:	09/01/2015
Certification File No.:	02156	Cert. Date:	09/01/2015
Linearity File No.:	02157	Lin. Date:	09/01/2015
Solution File No.:	02240	Soln. Date:	01/22/2016
Sequential File No.:	02340	File Date:	01/22/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK 53-0133
Control Solution %:	0.100%	Expires:	04/29/2016	Bottle No.:	1200
Solution Control Lot:	14D129				

Function	Result	Time	Temperature	Comments
	%BAC	HH-MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:165		
Control 1 EC	0.105%	14:168	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.105%	14:168	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	14:175		
Control 2 EC	0.104%	14:185	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	14:185	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:198		
Control 3 EC	0.104%	14:205	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	14:208	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:215		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NISP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:



Badge No.: 3200

Date: 01/22/2016

Calibrating Unit

New Standard Solution Report

Equipment	Alicon 7110 MSH-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT		
Calibration File No.	02155	Calib. Date:	08/01/2015
Certification File No.	02156	Cert. Date:	09/01/2015
Linearity File No.	02157	Lin. Date:	09/01/2015
Solution File No.	02239	Soln. Date:	01/22/2016
Sequential File No.	02239	File Date:	01/22/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DD17K S3-0133
Solution Control Lot:	15H149	Expires:	08/04/2017
		Bottle No.:	0165

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:07S		
Control 1 EC	---	13:08S	N/A	SIMULATOR TEMP. ERROR
Control 1 IR	---	13:08S	N/A	SIMULATOR TEMP. ERROR
Ambient Air Blank	---	---		
Control 2 EC	---	---	N/A	
Control 2 IR	---	---	N/A	
Ambient Air Blank	---	---		
Control 3 EC	---	---	N/A	
Control 3 IR	---	---	N/A	
Ambient Air Blank	---	---		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alicon 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 01/22/2016

