

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02772	Calib. Date: 10/07/2019
Certification File No.:	02773	Calib. No.: 00042
Linearity File No.:	02774	Cert. Date: 10/07/2019
Solution File No.:	02800	Lin. Date: 10/07/2019
Sequential File No.:	02800	Lin. No.: 00031
		Soln. Date: 12/21/2019
		Soln. No.: 00318
		File Date: 12/21/2019

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %: 0.100%		Expires: 06/10/2021
Solution Control Lot: 19150		Bottle No.: 0108

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:37S		
Control 1 EC	0.099%	04:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:39S		
Control 2 EC	0.098%	04:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:40S		
Control 3 EC	0.098%	04:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

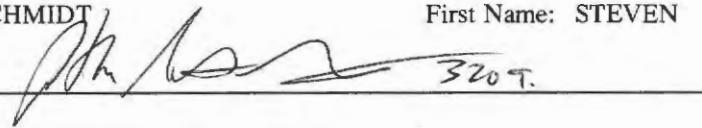

Badge No.: 3209

Date: 12/21/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02772	Calib. Date:	10/07/2019
Certification File No.:	02773	Cert. Date:	10/07/2019
Linearity File No.:	02774	Lin. Date:	10/07/2019
Solution File No.:	02790	Soln. Date:	11/28/2019
Sequential File No.:	02790	File Date:	11/28/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	19150	Expires:	06/10/2021
		Bottle No.:	0043

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:03S		
Control 1 EC	0.098%	05:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:04S		
Control 2 EC	0.098%	05:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	05:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:06S		
Control 3 EC	0.097%	05:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

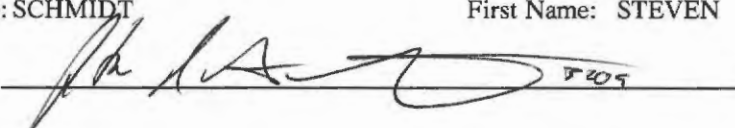

Badge No.: 3209

Date: 11/28/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02772	Calib. Date: 10/07/2019
Certification File No.:	02773	Cert. No.: 00042
Linearity File No.:	02774	Cert. Date: 10/07/2019
Solution File No.:	02787	Lin. No.: 00031
Sequential File No.:	02787	Soln. Date: 11/03/2019
		Soln. No.: 00316
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	0106	Expires: 06/10/2021
		Bottle No.: 0106

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:27S		
Control 1 EC	0.097%	11:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	11:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:28S		
Control 2 EC	0.096%	11:29S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	11:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:30S		
Control 3 EC	0.096%	11:30S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 11/03/2019

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 02772 Calib. Date: 10/07/2019 Calib. No.: 00042  
Certification File No.: 02773 Cert. Date: 10/07/2019 Cert. No.: 00032  
Linearity File No.: 02774 Lin. Date: 10/07/2019 Lin. No.: 00031  
Solution File No.: 02782 Soln. Date: 10/21/2019 Soln. No.: 00315  
Sequential File No.: 02782 File Date: 10/21/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
Control Solution %: 0.100% Expires: 06/10/2021  
Solution Control Lot: 19150 Bottle No.: 0211

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:53D		
Control 1 EC	0.099%	06:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:54D		
Control 2 EC	0.098%	06:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:56D		
Control 3 EC	0.098%	06:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:57D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: SCHMIDT

First Name: STEVEN

MI: D

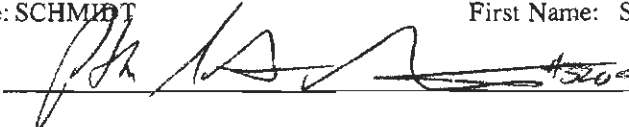Signature: 

Badge No.: 3209

Date: 10/21/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02721	Calib. Date: 05/10/2019
Certification File No.:	02722	Calb. No.: 00041
Linearity File No.:	02723	Cert. Date: 05/10/2019
Solution File No.:	02761	Cert. No.: 00031
Sequential File No.:	02761	Lin. Date: 05/10/2019
		Lin. No.: 00030
		Soln. Date: 09/20/2019
		Soln. No.: 00313
		File Date: 09/20/2019
<b>Calibrating Unit:</b>	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	18090	Expires: 03/13/2020
		Bottle No.: 0141

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:20D		
Control 1 EC	0.099%	19:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:21D		
Control 2 EC	0.097%	19:22D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:23D		
Control 3 EC	0.098%	19:23D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

Badge No.: 3209

Date: 09/20/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02721	Calib. Date: 05/10/2019
Certification File No.:	02722	Calib. No.: 00041
Linearity File No.:	02723	Cert. Date: 05/10/2019
Solution File No.:	02754	Cert. No.: 00031
Sequential File No.:	02754	Lin. Date: 05/10/2019
		Lin. No.: 00030
		Soln. Date: 08/29/2019
		Soln. No.: 00312
		File Date: 08/29/2019

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 03/13/2020
Solution Control Lot:	18090		Bottle No.: 0663

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:09D		
Control 1 EC	0.100%	15:10D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:11D		
Control 2 EC	0.098%	15:11D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:12D		
Control 3 EC	0.098%	15:13D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:14D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

*[Handwritten Signature]* 3200

Badge No.: 3200

Date: 08/29/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02721	Calib. Date:	05/10/2019
Certification File No.:	02722	Cert. Date:	05/10/2019
Linearity File No.:	02723	Lin. Date:	05/10/2019
Solution File No.:	02751	Soln. Date:	08/04/2019
Sequential File No.:	02751	File Date:	08/04/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	03/13/2020
Solution Control Lot:	18090			Bottle No.:	0073

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:20D		
Control 1 EC	0.099%	02:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:21D		
Control 2 EC	0.099%	02:22D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:23D		
Control 3 EC	0.099%	02:24D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3209

Date: 08/04/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02721	Calib. Date:	05/10/2019
Certification File No.:	02722	Cert. Date:	05/10/2019
Linearity File No.:	02723	Lin. Date:	05/10/2019
Solution File No.:	02746	Soln. Date:	07/14/2019
Sequential File No.:	02746	File Date:	07/14/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	03/13/2020
Solution Control Lot:	18090			Bottle No.:	0491

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:41D		
Control 1 EC	0.098%	00:42D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	00:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:43D		
Control 2 EC	0.097%	00:43D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:44D		
Control 3 EC	0.098%	00:45D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_

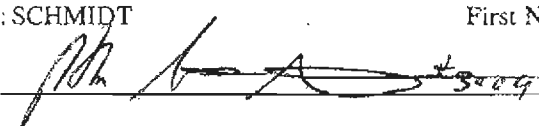

Badge No.: 3209

Date: 07/14/2019



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02721	Calib. Date:	05/10/2019
Certification File No.:	02722	Cert. Date:	05/10/2019
Linearity File No.:	02723	Lin. Date:	05/10/2019
Solution File No.:	02740	Soln. Date:	07/01/2019
Sequential File No.:	02740	File Date:	07/01/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0686

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:44D		
Control 1 EC	0.098%	02:45D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	02:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:46D		
Control 2 EC	0.097%	02:46D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:47D		
Control 3 EC	0.098%	02:48D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NISP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: 

Badge No.: 3209

Date: 07/01/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02721	Calib. Date: 05/10/2019
Certification File No.:	02722	Calib. No.: 00041
Linearity File No.:	02723	Cert. Date: 05/10/2019
Solution File No.:	02732	Cert. No.: 00031
Sequential File No.:	02732	Lin. Date: 05/10/2019
		Lin. No.: 00030
		Soln. Date: 06/05/2019
		Soln. No.: 00308
		File Date: 06/05/2019

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 03/13/2020
Solution Control Lot:	18090		Bottle No.: 0599

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:54D		
Control 1 EC	0.099%	03:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:55D		
Control 2 EC	0.099%	03:56D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:57D		
Control 3 EC	0.098%	03:57D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:58D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**


Last Name: SCHMIDT

First Name: STEVEN


MI: D

Signature:  SC10

Badge No.: 3210  
Date: 06/05/2019

Signature:  SC10

Badge No.: 3210  
Date: 06/05/2019

Signature:  SC10

Badge No.: 3210  
Date: 06/05/2019

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02647	Calib. Date:	11/29/2018
Certification File No.:	02648	Cert. Date:	11/29/2018
Linearity File No.:	02649	Lin. Date:	11/29/2018
Solution File No.:	02718	Soln. Date:	05/04/2019
Sequential File No.:	02718	File Date:	05/04/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0163
Control Solution %:	0.100%			Expires:	03/13/2020
Solution Control Lot:	18090			Bottle No.:	0368

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:21D		
Control 1 EC	0.104%	23:22D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:23D		
Control 2 EC	0.102%	23:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	23:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:24D		
Control 3 EC	0.103%	23:25D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	23:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D


Signature: \_\_\_\_\_

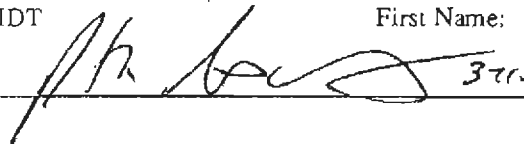

Badge No.: 3210

Date: 05/04/2019

Signature: \_\_\_\_\_



Badge No.: 3210

Date: 05/04/2019

Sequential File No.: 02718      File Date: 05/04/2019

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0163
Control Solution %:	0.100%			Expires:	03/13/2020
Solution Control Lot:	18090			Bottle No.:	0368

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:21D		
Control 1 EC	0.104%	23:22D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:23D		
Control 2 EC	0.102%	23:23D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	23:23D	33.9°C	*** TEST PASSED ***

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	02647	Calib. Date: 11/29/2018
Certification File No.:	02648	Calib. No.: 00040
Linearity File No.:	02649	Cert. Date: 11/29/2018
Solution File No.:	02717	Cert. No.: 00030
Sequential File No.:	02717	Lin. Date: 11/29/2018
		Lin. No.: 00029
		Soln. Date: 05/04/2019
		Soln. No.: 00305
		File Date: 05/04/2019
Calibrating Unit:	WET	Model No.: CU 34
Control Solution %:	0.100%	Serial No.: DDQL S3-0163
Solution Control Lot:	18090	Expires: 03/13/2020
		Bottle No.: 0355

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:07D		
Control 1 EC	0.104%	22:08D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	22:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:08D		
Control 2 EC	0.101%	22:09D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	22:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:10D		
Control 3 EC	0.103%	22:11D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.104%	22:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHMIDT

First Name: STEVEN

MI: D

Signature: \_\_\_\_\_



Badge No.: 3210

Date: 05/04/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment:</b> Alcotest 7110 MKIII-C	Serial No.: ARNK-0039	
<b>Location:</b> STRATFORD POLICE DEPT.		
Calibration File No.: 02647	Calib. Date: 11/29/2018	Calib. No.: 00040
Certification File No.: 02648	Cert. Date: 11/29/2018	Cert. No.: 00030
Linearity File No.: 02649	Lin. Date: 11/29/2018	Lin. No.: 00029
Solution File No.: 02707	Soln. Date: 04/07/2019	Soln. No.: 00304
Sequential File No.: 02707	File Date: 04/07/2019	
<b>Calibrating Unit:</b> WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %: 0.100%		Expires: 03/13/2020
Solution Control Lot: 18090		Bottle No.: 0355

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:56D		
Control 1 EC	0.101%	19:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.103%	19:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:58D		
Control 2 EC	0.100%	19:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.103%	19:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:59D		
Control 3 EC	0.100%	20:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	20:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_



#3201

Badge No.: 3201

Date: 04/07/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02647	Calib. Date:	11/29/2018
Certification File No.:	02648	Cert. Date:	11/29/2018
Linearity File No.:	02649	Lin. Date:	11/29/2018
Solution File No.:	02701	Soln. Date:	03/30/2019
Sequential File No.:	02701	File Date:	03/30/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0500

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:47S		
Control 1 EC	0.102%	09:47S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 2 EC	0.101%	09:49S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		
Control 3 EC	0.101%	09:50S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	09:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MOREL

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 03/30/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT	
Calibration File No.:	02647	Calib. Date: 11/29/2018
Certification File No.:	02648	Calib. No.: 00040
Linearity File No.:	02649	Cert. Date: 11/29/2018
Solution File No.:	02690	Cert. No.: 00030
Sequential File No.:	02690	Lin. Date: 11/29/2018
		Lin. No.: 00029
		Soln. Date: 03/02/2019
		Soln. No.: 00302
		File Date: 03/02/2019
<b>Calibrating Unit:</b>	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL-S3-0163
Solution Control Lot:	18090	Expires: 03/13/2020
		Bottle No.: 0578

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:01S		
Control 1 EC	0.103%	11:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03S		
Control 2 EC	0.102%	11:04S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		
Control 3 EC	0.101%	11:05S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	11:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63200

Badge No.: 3200

Date: 03/02/2019

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	02647	Calib. Date:	11/29/2018
Certification File No.:	02648	Cert. Date:	11/29/2018
Linearity File No.:	02649	Lin. Date:	11/29/2018
Solution File No.:	02683	Soln. Date:	02/06/2019
Sequential File No.:	02683	File Date:	02/06/2019
		Calib. No.:	00040
		Cert. No.:	00030
		Lin. No.:	00029
		Soln. No.:	00301
Calibrating Unit:	WET	Model No.:	CU-14
Control Solution %:	0.100%	Serial No.:	DDUL S3-0163
Solution Control Lot:	18090	Expires:	03/13/2020
		Bottle No.:	0682

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:49S		
Control 1 EC	0.102%	13:50S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51S		
Control 2 EC	0.101%	13:52S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52S		
Control 3 EC	0.100%	13:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	13:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: \_\_\_\_\_



Badge No.: 3201

Date: 02/06/2019



