

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARSB-0082
Location: GLASSBORO POLICE DEPT.
Calibration File No.: 00689 **Calib. Date:** 11/21/2008 **Calib. No.:** 00009
Certification File No.: 00690 **Cert. Date:** 11/21/2008 **Cert. No.:** 00007
Linearity File No.: 00691 **Lin. Date:** 11/21/2008 **Lin. No.:** 00007
Solution File No.: 00733 **Soln. Date:** 01/31/2009 **Soln. No.:** 00076
Sequential File No.: 00733 **File Date:** 01/31/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUD S3-0006
Control Solution %: 0.100% **Expires:** 07/23/2010
Solution Control Lot: 08G058 **Bottle No.:** 0516

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:39S		
Control 1 EC	0.100%	22:39S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:40S		
Control 2 EC	0.097%	22:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	22:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:42S		
Control 3 EC	0.099%	22:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____



Badge No.: 945

Date: 01/31/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSB-0082
Location:	GLASSBORO POLICE DEPT.	
Calibration File No.:	00689	Calib. Date: 11/21/2008
Certification File No.:	00690	Calib. No.: 00009
Linearity File No.:	00691	Cert. Date: 11/21/2008
Solution File No.:	00744	Cert. No.: 00007
Sequential File No.:	00744	Lin. Date: 11/21/2008
		Lin. No.: 00007
		Soln. Date: 02/14/2009
		Soln. No.: 00077
		File Date: 02/14/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0006
Solution Control Lot:	08G058	Expires: 07/23/2010
		Bottle No.: 1387

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:27S		
Control 1 EC	0.100%	07:28S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:29S		
Control 2 EC	0.097%	07:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:30S		
Control 3 EC	0.098%	07:31S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____

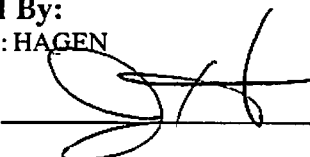

Badge No.: 945

Date: 02/14/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSB-0082
Location:	GLASSBORO POLICE DEPT.	
Calibration File No.:	00689	Calib. Date: 11/21/2008
Certification File No.:	00690	Calib. No.: 00009
Linearity File No.:	00691	Cert. Date: 11/21/2008
Solution File No.:	00750	Cert. No.: 00007
Sequential File No.:	00750	Lin. Date: 11/21/2008
		Lin. No.: 00007
		Soln. Date: 03/04/2009
		Soln. No.: 00078
		File Date: 03/04/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0006
Solution Control Lot:	08G058	Expires: 07/23/2010
		Bottle No.: 0521

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:54S		
Control 1 EC	0.100%	15:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:55S		
Control 2 EC	0.097%	15:56S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:57S		
Control 3 EC	0.098%	15:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:58S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____

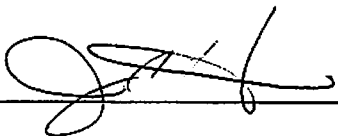

Badge No.: 945

Date: 03/04/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSB-0082
Location:	GLASSBORO POLICE DEPT.	
Calibration File No.:	00689	Calib. Date: 11/21/2008
Certification File No.:	00690	Calib. No.: 00009
Linearity File No.:	00691	Cert. Date: 11/21/2008
Solution File No.:	00759	Cert. No.: 00007
Sequential File No.:	00759	Lin. Date: 11/21/2008
		Lin. No.: 00007
		Soln. Date: 03/22/2009
		Soln. No.: 00079
		File Date: 03/22/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0006
Solution Control Lot:	08G058	Expires: 07/23/2010
		Bottle No.: 0517

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:44S		
Control 1 EC	0.100%	18:45S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:45S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:46S		
Control 2 EC	0.099%	18:46S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:47S		
Control 3 EC	0.098%	18:48S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____



Badge No.: 945

Date: 03/22/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSB-0082
Location:	GLASSBORO POLICE DEPT.	
Calibration File No.:	00689	Calib. Date: 11/21/2008
Certification File No.:	00690	Calib. No.: 00009
Linearity File No.:	00691	Cert. Date: 11/21/2008
Solution File No.:	00765	Cert. No.: 00007
Sequential File No.:	00765	Lin. Date: 11/21/2008
		Lin. No.: 00007
		Soln. Date: 04/08/2009
		Soln. No.: 00080
		File Date: 04/08/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUD S3-0006
Solution Control Lot:	08G058	Expires: 07/23/2010
		Bottle No.: 0524

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:36D		
Control 1 EC	0.100%	03:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:37D		
Control 2 EC	0.099%	03:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:39D		
Control 3 EC	0.099%	03:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____



Badge No.: 945

Date: 04/08/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARSB-0082
Location: GLASSBORO POLICE DEPT.
Calibration File No.: 00768 Calib. Date: 04/13/2009 Calib. No.: 00010
Certification File No.: 00769 Cert. Date: 04/13/2009 Cert. No.: 00008
Linearity File No.: 00770 Lin. Date: 04/13/2009 Lin. No.: 00008
Solution File No.: 00785 Soln. Date: 05/05/2009 Soln. No.: 00082
Sequential File No.: 00785 File Date: 05/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUD S3-0007
Control Solution %: 0.100% Expires: 07/23/2010
Solution Control Lot: 08G058 Bottle No.: 0514

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:18D		
Control 1 EC	0.099%	13:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		
Control 2 EC	0.098%	13:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21D		
Control 3 EC	0.098%	13:22D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:22D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HAGEN

First Name: JOHN

MI: C

Signature: _____



Badge No.: 945

Date: 05/05/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARSB-0082
Location:	GLASSBORO POLICE DEPT.	
Calibration File No.:	00768	Calib. Date: 04/13/2009
Certification File No.:	00769	Calib. No.: 00010
Linearity File No.:	00770	Cert. Date: 04/13/2009
Solution File No.:	00795	Cert. No.: 00008
Sequential File No.:	00795	Lin. Date: 04/13/2009
		Lin. No.: 00008
		Soln. Date: 05/25/2009
		Soln. No.: 00083
		File Date: 05/25/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUD S3-0007
Control Solution %:	0.100%		Expires: 07/23/2010
Solution Control Lot:	08G058		Bottle No.: 0523

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:20D		
Control 1 EC	0.100%	07:20D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	07:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:21D		
Control 2 EC	0.099%	07:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:23D		
Control 3 EC	0.099%	07:23D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HERNER

First Name: CHRISTOPHER

MI: B

Signature: _____

Mr. Cliff B. R. #960

Badge No.: 960

Date: 05/25/2009