

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00005	Calib. Date: 10/20/2005
Certification File No.:	00006	Calib. No.: 00002
Linearity File No.:	00007	Cert. Date: 10/20/2005
Solution File No.:	00008	Cert. No.: 00001
Sequential File No.:	00008	Lin. Date: 10/20/2005
		Lin. No.: 00001
		Soln. Date: 10/20/2005
		Soln. No.: 00003
		File Date: 10/20/2005

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0166
Control Solution %:	0.100%		Expires: 04/14/2007
Solution Control Lot:	05D017		Bottle No.: 0293

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:05D		
Control 1 EC	0.100%	11:06D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:06D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 2 EC	0.100%	11:07D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		
Control 3 EC	0.099%	11:08D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:08D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: _____

TPR. I WILL M. Cross #5342

Badge No.: 5342

Date: 10/20/2005

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00005	Calib. Date: 10/20/2005
Certification File No.:	00006	Cert. No.: 00002
Linearity File No.:	00007	Cert. Date: 10/20/2005
Solution File No.:	00016	Lin. No.: 00001
Sequential File No.:	00016	Lin. Date: 10/20/2005
		Soln. No.: 00004
		Soln. Date: 11/18/2005
		File Date: 11/18/2005
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0166
Solution Control Lot:	05D017	Expires: 04/14/2007
		Bottle No.: 0351

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:27S		
Control 1 EC	0.098%	09:27S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:27S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28S		
Control 2 EC	0.098%	09:28S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:28S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29S		
Control 3 EC	0.098%	09:30S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:30S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: Kevin Shoppas

Badge No.: 3046

Date: 11/18/2005

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00022 **Soln. Date:** 12/19/2005 **Soln. No.:** 00005
Sequential File No.: 00022 **File Date:** 12/19/2005

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0251

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:18S		
Control 1 EC	0.099%	08:18S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:18S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19S		
Control 2 EC	0.098%	08:19S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20S		
Control 3 EC	0.098%	08:21S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:21S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:22S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: 

Badge No.: 3046

Date: 12/19/2005

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00029 **Soln. Date:** 01/16/2006 **Soln. No.:** 00006
Sequential File No.: 00029 **File Date:** 01/16/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0254

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:52S		
Control 1 EC	0.098%	08:52S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53S		
Control 2 EC	0.098%	08:54S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:54S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:54S		
Control 3 EC	0.098%	08:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: Sgt Kevin Shoppas

Badge No.: 3046

Date: 01/16/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00040 **Soln. Date:** 02/07/2006 **Soln. No.:** 00007
Sequential File No.: 00040 **File Date:** 02/07/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0260

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:17S		
Control 1 EC	0.100%	04:17S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:17S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:18S		
Control 2 EC	0.099%	04:19S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:19S		
Control 3 EC	0.100%	04:20S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:20S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: Sgt. K. Shoppas

Badge No.: 3046

Date: 02/07/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00005	Calib. Date: 10/20/2005
Certification File No.:	00006	Calib. No.: 00002
Linearity File No.:	00007	Cert. Date: 10/20/2005
Solution File No.:	00051	Cert. No.: 00001
Sequential File No.:	00051	Lin. Date: 10/20/2005
		Lin. No.: 00001
		Soln. Date: 03/15/2006
		Soln. No.: 00008
		File Date: 03/15/2006

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0166
Solution Control Lot:	05D017	Expires: 04/14/2007
		Bottle No.: 0356

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:06S		
Control 1 EC	0.099%	12:06S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:06S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		
Control 2 EC	0.099%	12:08S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:08S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:08S		
Control 3 EC	0.098%	12:09S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:09S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: Sgt Kevin A. Shoppas

Badge No.: 3046

Date: 03/15/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00060 **Soln. Date:** 04/15/2006 **Soln. No.:** 00010
Sequential File No.: 00060 **File Date:** 04/15/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0353

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:40D		
Control 1 EC	0.100%	19:40D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:41D		
Control 2 EC	0.099%	19:42D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:42D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:42D		
Control 3 EC	0.099%	19:43D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:43D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: 

Badge No.: 3045

Date: 04/15/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00066 **Soln. Date:** 05/22/2006 **Soln. No.:** 00011
Sequential File No.: 00066 **File Date:** 05/22/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0286

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:04D		
Control 1 EC	0.099%	14:04D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:04D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 2 EC	0.099%	14:05D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:05D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:06D		
Control 3 EC	0.098%	14:07D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: _____



Badge No.: 3045

Date: 05/22/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 Calib. Date: 10/20/2005 Calib. No.: 00002
Certification File No.: 00006 Cert. Date: 10/20/2005 Cert. No.: 00001
Linearity File No.: 00007 Lin. Date: 10/20/2005 Lin. No.: 00001
Solution File No.: 00070 Soln. Date: 06/21/2006 Soln. No.: 00012
Sequential File No.: 00070 File Date: 06/21/2006

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 04/14/2007
Solution Control Lot: 05D017 Bottle No.: 0352

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:17D		
Control 1 EC	0.099%	05:18D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:19D		
Control 2 EC	0.099%	05:19D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:19D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:20D		
Control 3 EC	0.099%	05:20D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:20D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: 

Badge No.: 3045

Date: 06/21/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 Calib. Date: 10/20/2005 Calib. No.: 00002
Certification File No.: 00006 Cert. Date: 10/20/2005 Cert. No.: 00001
Linearity File No.: 00007 Lin. Date: 10/20/2005 Lin. No.: 00001
Solution File No.: 00081 Soln. Date: 07/27/2006 Soln. No.: 00013
Sequential File No.: 00081 File Date: 07/27/2006

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 04/14/2007
Solution Control Lot: 05D017 Bottle No.: 0281

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:09D		
Control 1 EC	0.098%	06:09D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:09D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:10D		
Control 2 EC	0.098%	06:11D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:11D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:11D		
Control 3 EC	0.097%	06:12D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:12D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: 

Badge No.: 3045

Date: 07/27/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00005	Calib. Date: 10/20/2005
Certification File No.:	00006	Cert. No.: 00002
Linearity File No.:	00007	Cert. Date: 10/20/2005
Solution File No.:	00093	Lin. Date: 10/20/2005
Sequential File No.:	00093	Lin. No.: 00001
		Soln. Date: 08/21/2006
		Soln. No.: 00015
		File Date: 08/21/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0166
Solution Control Lot:	05D017	Expires: 04/14/2007
		Bottle No.: 0360

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:45D		
Control 1 EC	0.100%	13:46D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:46D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47D		
Control 2 EC	0.098%	13:47D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:47D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:48D		
Control 3 EC	0.097%	13:49D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:49D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:			
Last Name:	CARNIVALE	First Name:	MARC
Signature:			MI: A
		Badge No.:	60
		Date:	08/21/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00005 **Calib. Date:** 10/20/2005 **Calib. No.:** 00002
Certification File No.: 00006 **Cert. Date:** 10/20/2005 **Cert. No.:** 00001
Linearity File No.: 00007 **Lin. Date:** 10/20/2005 **Lin. No.:** 00001
Solution File No.: 00104 **Soln. Date:** 09/20/2006 **Soln. No.:** 00016
Sequential File No.: 00104 **File Date:** 09/20/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0354

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:53D		
Control 1 EC	0.099%	13:54D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:54D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:55D		
Control 2 EC	0.099%	13:55D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:55D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:56D		
Control 3 EC	0.097%	13:56D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:56D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

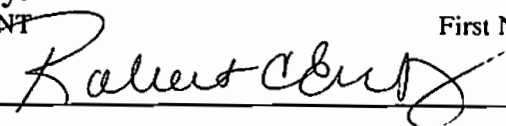
Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: _____



Badge No.: 3045

Date: 09/20/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00106 **Calib. Date:** 10/12/2006 **Calib. No.:** 00003
Certification File No.: 00107 **Cert. Date:** 10/12/2006 **Cert. No.:** 00002
Linearity File No.: 00108 **Lin. Date:** 10/12/2006 **Lin. No.:** 00002
Solution File No.: 00109 **Soln. Date:** 10/12/2006 **Soln. No.:** 00017
Sequential File No.: 00109 **File Date:** 10/12/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0167
Control Solution %: 0.100% **Expires:** 04/14/2007
Solution Control Lot: 05D017 **Bottle No.:** 0252

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:11D		
Control 1 EC	0.099%	11:12D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:12D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13D		
Control 2 EC	0.099%	11:13D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:13D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:14D		
Control 3 EC	0.099%	11:14D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:14D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDXP2-011 WML

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: TPR. I WILL M. Cross #5342

Badge No.: 5342

Date: 10/12/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD		
Calibration File No.:	00106	Calib. Date:	10/12/2006
Certification File No.:	00107	Cert. No.:	00003
Linearity File No.:	00108	Cert. Date:	10/12/2006
Solution File No.:	00119	Lin. No.:	00002
Sequential File No.:	00119	Lin. Date:	10/12/2006
		Soln. No.:	00018
		Soln. Date:	11/12/2006
		File Date:	11/12/2006
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0167
Solution Control Lot:	05D017	Expires:	04/14/2007
		Bottle No.:	0276

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:56S		
Control 1 EC	0.100%	00:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:57S		
Control 2 EC	0.099%	00:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:58S		
Control 3 EC	0.099%	00:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

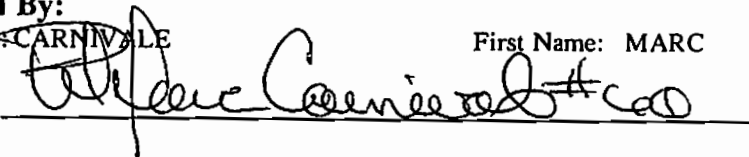
Changed By:

Last Name: CARNIVALE

First Name: MARC

MI: A

Signature:



Badge No.: 60

Date: 11/12/2006

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00106 Calib. Date: 10/12/2006 Calib. No.: 00003
Certification File No.: 00107 Cert. Date: 10/12/2006 Cert. No.: 00002
Linearity File No.: 00108 Lin. Date: 10/12/2006 Lin. No.: 00002
Solution File No.: 00128 Soln. Date: 12/10/2006 Soln. No.: 00019
Sequential File No.: 00128 File Date: 12/10/2006

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0167
Control Solution %: 0.100% Expires: 07/20/2008
Solution Control Lot: 06G034 Bottle No.: 0193

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:46S		
Control 1 EC	0.099%	21:46S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:46S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:47S		
Control 2 EC	0.099%	21:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:48S		
Control 3 EC	0.099%	21:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature:  #45

Badge No.: 3045

Date: 12/10/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00196 **Calib. Date:** 10/04/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/04/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/04/2007 **Lin. No.:** 00003
Solution File No.: 00233 **Soln. Date:** 01/21/2008 **Soln. No.:** 00035
Sequential File No.: 00233 **File Date:** 01/21/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 07/20/2008
Solution Control Lot: 06G034 **Bottle No.:** 0184

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:36S		
Control 1 EC	0.099%	15:36S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:36S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:37S		
Control 2 EC	0.099%	15:38S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:39S		
Control 3 EC	0.099%	15:39S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:40S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 01/21/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD		
Calibration File No.:	00196	Calib. Date:	10/04/2007
Certification File No.:	00197	Cert. No.:	00004
Linearity File No.:	00198	Cert. Date:	10/04/2007
Solution File No.:	00237	Lin. Date:	10/04/2007
Sequential File No.:	00237	Lin. No.:	00003
		Soln. Date:	02/18/2008
		Soln. No.:	00036
		File Date:	02/18/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0166
Solution Control Lot:	06G034	Expires:	07/20/2008
		Bottle No.:	0177

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:07S		
Control 1 EC	0.100%	16:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:09S		
Control 2 EC	0.099%	16:09S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:09S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:10S		
Control 3 EC	0.099%	16:10S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	16:10S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

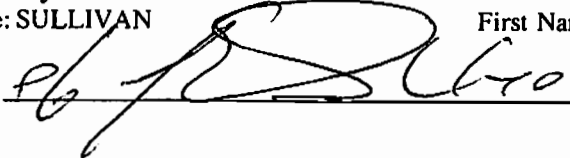
Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 02/18/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00196 **Calib. Date:** 10/04/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/04/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/04/2007 **Lin. No.:** 00003
Solution File No.: 00247 **Soln. Date:** 03/18/2008 **Soln. No.:** 00037
Sequential File No.: 00247 **File Date:** 03/18/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 07/20/2008
Solution Control Lot: 06G034 **Bottle No.:** 0186

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:43S		
Control 1 EC	0.099%	19:43S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:43S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:44S		
Control 2 EC	0.096%	19:45S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:45S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:46S		
Control 3 EC	0.097%	19:46S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:46S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:47S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

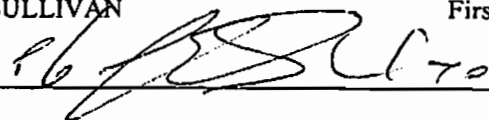
Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 03/18/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00196 **Calib. Date:** 10/04/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/04/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/04/2007 **Lin. No.:** 00003
Solution File No.: 00258 **Soln. Date:** 04/06/2008 **Soln. No.:** 00038
Sequential File No.: 00258 **File Date:** 04/06/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 07/20/2008
Solution Control Lot: 06G034 **Bottle No.:** 0188

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:13D		
Control 1 EC	0.096%	10:13D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:13D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14D		
Control 2 EC	0.091%	10:15D	34.1°C	CONTROL TEST FAILED
Control 2 IR	0.092%	10:15D	34.1°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	10:15D		
Control 3 EC	0.094%	10:16D	34.1°C	CONTROL TEST FAILED
Control 3 IR	0.094%	10:16D	34.1°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	10:17D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 04/06/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00196 **Calib. Date:** 10/04/2007 **Calib. No.:** 00004
Certification File No.: 00197 **Cert. Date:** 10/04/2007 **Cert. No.:** 00003
Linearity File No.: 00198 **Lin. Date:** 10/04/2007 **Lin. No.:** 00003
Solution File No.: 00259 **Soln. Date:** 04/06/2008 **Soln. No.:** 00039
Sequential File No.: 00259 **File Date:** 04/06/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0166
Control Solution %: 0.100% **Expires:** 07/20/2008
Solution Control Lot: 06G034 **Bottle No.:** 0200

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:06D		
Control 1 EC	0.097%	15:07D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.098%	15:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:08D		
Control 2 EC	0.095%	15:08D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:08D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:09D		
Control 3 EC	0.097%	15:10D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	15:10D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:10D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 04/06/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00263 **Calib. Date:** 04/29/2008 **Calib. No.:** 00005
Certification File No.: 00264 **Cert. Date:** 04/29/2008 **Cert. No.:** 00004
Linearity File No.: 00265 **Lin. Date:** 04/29/2008 **Lin. No.:** 00004
Solution File No.: 00266 **Soln. Date:** 04/29/2008 **Soln. No.:** 00040
Sequential File No.: 00266 **File Date:** 04/29/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0167
Control Solution %: 0.100% **Expires:** 07/20/2008
Solution Control Lot: 06G034 **Bottle No.:** 0182

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:50D		
Control 1 EC	0.100%	11:50D	34.1 °C	*** TEST PASSED ***
Control 1 IR	0.100%	11:50D	34.1 °C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51D		
Control 2 EC	0.100%	11:52D	34.1 °C	*** TEST PASSED ***
Control 2 IR	0.100%	11:52D	34.1 °C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52D		
Control 3 EC	0.099%	11:53D	34.1 °C	*** TEST PASSED ***
Control 3 IR	0.099%	11:53D	34.1 °C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDXAP2-011 WR

Changed By:

Last Name: CROSS

First Name: WILLIAM

MI: M

Signature: TPR. I WILLIAM. Cross #5342

Badge No.: 5342

Date: 04/29/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	Calib. No.:	00005
Calibration File No.:	00263	Cert. Date:	04/29/2008
Certification File No.:	00264	Lin. Date:	04/29/2008
Linearity File No.:	00265	Soln. Date:	05/03/2008
Solution File No.:	00269	File Date:	05/03/2008
Sequential File No.:	00269		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0167
Solution Control Lot:	06G034	Expires:	07/20/2008
		Bottle No.:	0196

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:26D		
Control 1 EC	0.100%	18:27D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:27D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:28D		
Control 2 EC	0.099%	18:28D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:28D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:29D		
Control 3 EC	0.099%	18:29D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:29D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:30D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

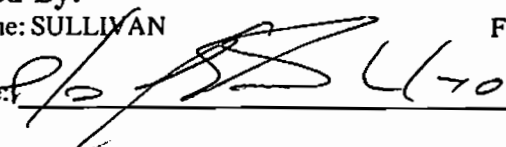
Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 05/03/2008



Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00263	Calib. Date: 04/29/2008
Certification File No.:	00264	Cert. No.: 00005
Linearity File No.:	00265	Cert. Date: 04/29/2008
Solution File No.:	00292	Lin. No.: 00004
Sequential File No.:	00292	Soln. No.: 00043
		File Date: 07/09/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0167
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0033

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:15D		
Control 1 EC	0.101%	17:16D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:16D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:17D		
Control 2 EC	0.101%	17:17D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	17:17D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:18D		
Control 3 EC	0.100%	17:18D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 07/09/2008



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 06/23/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B046

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 24, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 13th day of July, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



F-7/18/08

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00263 Calib. Date: 04/29/2008 Calib. No.: 00005
Certification File No.: 00264 Cert. Date: 04/29/2008 Cert. No.: 00004
Linearity File No.: 00265 Lin. Date: 04/29/2008 Lin. No.: 00004
Solution File No.: 00299 Soln. Date: 08/08/2008 Soln. No.: 00044
Sequential File No.: 00299 File Date: 08/08/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0167
Control Solution %: 0.100% Expires: 10/03/2009
Solution Control Lot: 07J048 Bottle No.: 1258

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:48D		
Control 1 EC	0.099%	23:49D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:49D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50D		
Control 2 EC	0.099%	23:50D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:50D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:51D		
Control 3 EC	0.099%	23:52D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:52D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 08/08/2008



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 11/28/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07J048

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1225 to 0.1229 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 17th day of December, 2007.

Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00263 Calib. Date: 04/29/2008 Calib. No.: 00005
Certification File No.: 00264 Cert. Date: 04/29/2008 Cert. No.: 00004
Linearity File No.: 00265 Lin. Date: 04/29/2008 Lin. No.: 00004
Solution File No.: 00318 Soln. Date: 09/07/2008 Soln. No.: 00045
Sequential File No.: 00318 File Date: 09/07/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0167
Control Solution %: 0.100% Expires: 10/03/2009
Solution Control Lot: 07J048 Bottle No.: 1260

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:26D		
Control 1 EC	0.100%	01:27D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	01:27D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:27D		
Control 2 EC	0.099%	01:28D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:28D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:29D		
Control 3 EC	0.099%	01:29D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:29D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:30D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 09/07/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00263 **Calib. Date:** 04/29/2008 **Calib. No.:** 00005
Certification File No.: 00264 **Cert. Date:** 04/29/2008 **Cert. No.:** 00004
Linearity File No.: 00265 **Lin. Date:** 04/29/2008 **Lin. No.:** 00004
Solution File No.: 00324 **Soln. Date:** 10/08/2008 **Soln. No.:** 00046
Sequential File No.: 00324 **File Date:** 10/08/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0167
Control Solution %: 0.100% **Expires:** 06/09/2010
Solution Control Lot: 08F053 **Bottle No.:** 0503

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:07D		
Control 1 EC	0.100%	09:08D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:08D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:09D		
Control 2 EC	0.099%	09:09D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:09D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:10D		
Control 3 EC	0.100%	09:10D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:10D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 10/08/2008



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

ANNE MILORAM
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 07/03/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F053

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1238 to 0.1242 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 9, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 25th day of July, 2008.

Linda L. DeSantis
 Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD		
Calibration File No.:	00325	Calib. Date:	10/24/2008
Certification File No.:	00326	Cert. No.:	00006
Linearity File No.:	00327	Cert. Date:	10/24/2008
Solution File No.:	00337	Lin. No.:	00005
Sequential File No.:	00337	Soln. Date:	11/22/2008
		Soln. No.:	00048
		File Date:	11/22/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0167
Solution Control Lot:	08F053	Expires:	06/09/2010
		Bottle No.:	0518

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:14S		
Control 1 EC	0.100%	12:14S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:14S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15S		
Control 2 EC	0.099%	12:16S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:16S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16S		
Control 3 EC	0.099%	12:17S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:17S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SHOPPAS

First Name: KEVIN

MI: -

Signature: *Sgt. Kevin Shoppas*

Badge No.: 3046

Date: 11/22/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00325 Calib. Date: 10/24/2008 Calib. No.: 00006
Certification File No.: 00326 Cert. Date: 10/24/2008 Cert. No.: 00005
Linearity File No.: 00327 Lin. Date: 10/24/2008 Lin. No.: 00005
Solution File No.: 00345 Soln. Date: 12/22/2008 Soln. No.: 00049
Sequential File No.: 00345 File Date: 12/22/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0167
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0513

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:19S		
Control 1 EC	0.100%	12:19S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:20S		
Control 2 EC	0.099%	12:21S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:21S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		
Control 3 EC	0.099%	12:22S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:22S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

M1: B

Signature: 

Badge No.: 70

Date: 12/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00325	Calib. Date: 10/24/2008
Certification File No.:	00326	Calib. No.: 00006
Linearity File No.:	00327	Cert. Date: 10/24/2008
Solution File No.:	00354	Cert. No.: 00005
Sequential File No.:	00354	Lin. Date: 10/24/2008
		Lin. No.: 00005
		Soln. Date: 01/20/2009
		Soln. No.: 00050
		File Date: 01/20/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0167
Solution Control Lot:	08F053	Expires: 06/09/2010
		Bottle No.: 0521

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:47S		
Control 1 EC	0.100%	20:48S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:48S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:49S		
Control 2 EC	0.101%	20:49S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:49S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:50S		
Control 3 EC	0.100%	20:51S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:51S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:52S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 01/20/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD		
Calibration File No.:	00325	Calib. Date:	10/24/2008
Certification File No.:	00326	Cert. No.:	00006
Linearity File No.:	00327	Cert. Date:	10/24/2008
Solution File No.:	00364	Lin. No.:	00005
Sequential File No.:	00364	Soln. Date:	02/09/2009
		Soln. No.:	00051
		File Date:	02/09/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0167
Solution Control Lot:	08F053	Expires:	06/09/2010
		Bottle No.:	0011

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:46S		
Control 1 EC	0.102%	09:47S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:47S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 2 EC	0.101%	09:49S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:49S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49S		
Control 3 EC	0.101%	09:50S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:50S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: 00XAP2-011 FTL

Changed By:

Last Name: MASSENBERG

First Name: FERNANDEZ

MI: -

Signature: *[Handwritten Signature]* 5623

Badge No.: 5623

Date: 02/09/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00325 **Calib. Date:** 10/24/2008 **Calib. No.:** 00006
Certification File No.: 00326 **Cert. Date:** 10/24/2008 **Cert. No.:** 00005
Linearity File No.: 00327 **Lin. Date:** 10/24/2008 **Lin. No.:** 00005
Solution File No.: 00367 **Soln. Date:** 03/02/2009 **Soln. No.:** 00053
Sequential File No.: 00367 **File Date:** 03/02/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0167
Control Solution %: 0.100% **Expires:** 06/09/2010
Solution Control Lot: 08F053 **Bottle No.:** 0508

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:59S		
Control 1 EC	0.100%	17:59S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:59S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:00S		
Control 2 EC	0.100%	18:01S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:01S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:02S		
Control 3 EC	0.100%	18:02S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:02S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 03/02/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0024
Location:	BURLINGTON TOWNSHIP PD	
Calibration File No.:	00368	Calib. Date: 03/10/2009
Certification File No.:	00369	Calib. No.: 00007
Linearity File No.:	00370	Cert. Date: 03/10/2009
Solution File No.:	00378	Cert. No.: 00006
Sequential File No.:	00378	Lin. Date: 03/10/2009
		Lin. No.: 00006
		Soln. Date: 04/02/2009
		Soln. No.: 00055
		File Date: 04/02/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0166
Solution Control Lot:	08F053	Expires: 06/09/2010
		Bottle No.: 1400

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:13S		
Control 1 EC	0.099%	22:14S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	22:14S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:14S		
Control 2 EC	0.099%	22:15S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	22:15S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:16S		
Control 3 EC	0.099%	22:16S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:16S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:17S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HAZZARD

First Name: FLOYD

MI: M

Signature: _____



Badge No.: 72

Date: 04/02/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00368 Calib. Date: 03/10/2009 Calib. No.: 00007
Certification File No.: 00369 Cert. Date: 03/10/2009 Cert. No.: 00006
Linearity File No.: 00370 Lin. Date: 03/10/2009 Lin. No.: 00006
Solution File No.: 00385 Soln. Date: 04/24/2009 Soln. No.: 00056
Sequential File No.: 00385 File Date: 04/24/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0522

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:33D		
Control 1 EC	0.099%	01:33D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:33D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:34D		
Control 2 EC	0.098%	01:34D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:34D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:35D		
Control 3 EC	0.099%	01:36D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	01:36D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENT

First Name: ROBERT

MI: C

Signature: 

Badge No.: 3045

Date: 04/24/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00368 Calib. Date: 03/10/2009 Calib. No.: 00007
Certification File No.: 00369 Cert. Date: 03/10/2009 Cert. No.: 00006
Linearity File No.: 00370 Lin. Date: 03/10/2009 Lin. No.: 00006
Solution File No.: 00393 Soln. Date: 05/26/2009 Soln. No.: 00057
Sequential File No.: 00393 File Date: 05/26/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0613

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:03D		
Control 1 EC	0.099%	00:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	00:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:04D		
Control 2 EC	0.098%	00:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:06D		
Control 3 EC	0.098%	00:06D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:06D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: _____



Badge No.: 70

Date: 05/26/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00368 Calib. Date: 03/10/2009 Calib. No.: 00007
Certification File No.: 00369 Cert. Date: 03/10/2009 Cert. No.: 00006
Linearity File No.: 00370 Lin. Date: 03/10/2009 Lin. No.: 00006
Solution File No.: 00398 Soln. Date: 06/20/2009 Soln. No.: 00058
Sequential File No.: 00398 File Date: 06/20/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0505

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:23D		
Control 1 EC	0.098%	14:24D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:24D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:25D		
Control 2 EC	0.097%	14:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:26D		
Control 3 EC	0.097%	14:27D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:27D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:27D		

All tests within acceptable tolerance.

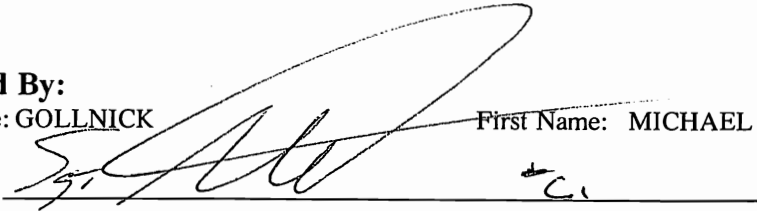
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 06/20/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00368 Calib. Date: 03/10/2009 Calib. No.: 00007
Certification File No.: 00369 Cert. Date: 03/10/2009 Cert. No.: 00006
Linearity File No.: 00370 Lin. Date: 03/10/2009 Lin. No.: 00006
Solution File No.: 00406 Soln. Date: 07/05/2009 Soln. No.: 00060
Sequential File No.: 00406 File Date: 07/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0510

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:54D		
Control 1 EC	0.098%	09:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		
Control 2 EC	0.098%	09:56D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:56D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57D		
Control 3 EC	0.098%	09:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:58D		

All tests within acceptable tolerance.

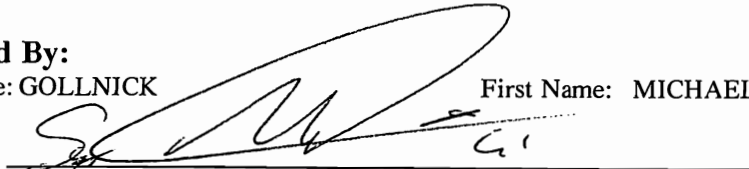
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 07/05/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00368 Calib. Date: 03/10/2009 Calib. No.: 00007
Certification File No.: 00369 Cert. Date: 03/10/2009 Cert. No.: 00006
Linearity File No.: 00370 Lin. Date: 03/10/2009 Lin. No.: 00006
Solution File No.: 00411 Soln. Date: 08/03/2009 Soln. No.: 00061
Sequential File No.: 00411 File Date: 08/03/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0514

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:14D		
Control 1 EC	0.099%	05:15D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:15D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:16D		
Control 2 EC	0.098%	05:16D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:16D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:17D		
Control 3 EC	0.098%	05:18D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:18D		

All tests within acceptable tolerance.

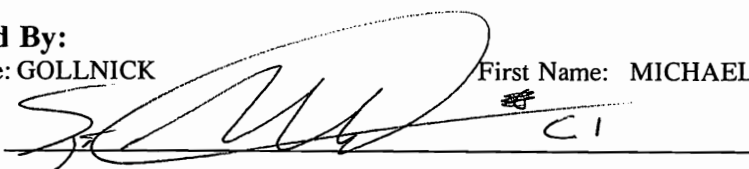
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 08/03/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0024
Location:	BURLINGTON TOWNSHIP PD		
Calibration File No.:	00417	Calib. Date:	08/25/2009
Certification File No.:	00418	Cert. No.:	00008
Linearity File No.:	00419	Cert. Date:	08/25/2009
Solution File No.:	00420	Lin. No.:	00007
Sequential File No.:	00420	Soln. Date:	08/25/2009
		Soln. No.:	00062
		File Date:	08/25/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0166
Solution Control Lot:	08F053	Expires:	06/09/2010
		Bottle No.:	0523

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:11D		
Control 1 EC	0.101%	13:12D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:12D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:12D		
Control 2 EC	0.100%	13:13D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:13D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:14D		
Control 3 EC	0.100%	13:14D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:14D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUSP2-025 FM

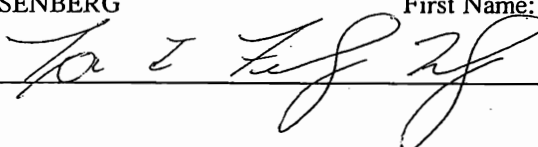
Changed By:

Last Name: MASSENBERG

First Name: FERNANDEZ

MI: -

Signature: _____



Badge No.: 5623

Date: 08/25/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00417 Calib. Date: 08/25/2009 Calib. No.: 00008
Certification File No.: 00418 Cert. Date: 08/25/2009 Cert. No.: 00007
Linearity File No.: 00419 Lin. Date: 08/25/2009 Lin. No.: 00007
Solution File No.: 00426 Soln. Date: 09/24/2009 Soln. No.: 00063
Sequential File No.: 00426 File Date: 09/24/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0519

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:05D		
Control 1 EC	0.100%	04:06D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:06D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:06D		
Control 2 EC	0.099%	04:07D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:07D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:08D		
Control 3 EC	0.099%	04:08D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:08D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: WENGER

First Name: KAREN

MI: M

Signature: *P/O K Wenger 75*

Badge No.: 3075

Date: 09/24/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00417 Calib. Date: 08/25/2009 Calib. No.: 00008
Certification File No.: 00418 Cert. Date: 08/25/2009 Cert. No.: 00007
Linearity File No.: 00419 Lin. Date: 08/25/2009 Lin. No.: 00007
Solution File No.: 00435 Soln. Date: 10/24/2009 Soln. No.: 00064
Sequential File No.: 00435 File Date: 10/24/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0506

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:47D		
Control 1 EC	0.099%	08:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49D		
Control 2 EC	0.099%	08:49D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:49D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50D		
Control 3 EC	0.099%	08:51D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:51D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:52D		

All tests within acceptable tolerance.

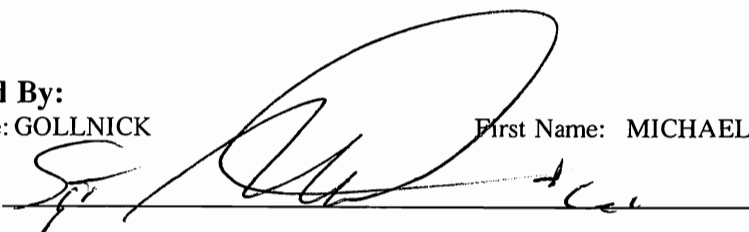
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 10/24/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00417 Calib. Date: 08/25/2009 Calib. No.: 00008
Certification File No.: 00418 Cert. Date: 08/25/2009 Cert. No.: 00007
Linearity File No.: 00419 Lin. Date: 08/25/2009 Lin. No.: 00007
Solution File No.: 00445 Soln. Date: 11/21/2009 Soln. No.: 00065
Sequential File No.: 00445 File Date: 11/21/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0524

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:46S		
Control 1 EC	0.100%	17:46S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:46S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:47S		
Control 2 EC	0.099%	17:48S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:48S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:48S		
Control 3 EC	0.099%	17:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:50S		

All tests within acceptable tolerance.

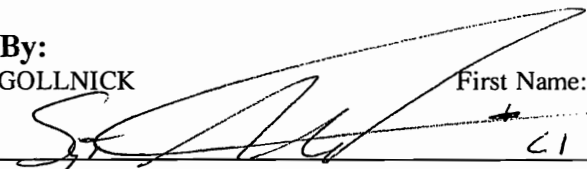
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 11/21/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00417 Calib. Date: 08/25/2009 Calib. No.: 00008
Certification File No.: 00418 Cert. Date: 08/25/2009 Cert. No.: 00007
Linearity File No.: 00419 Lin. Date: 08/25/2009 Lin. No.: 00007
Solution File No.: 00452 Soln. Date: 12/06/2009 Soln. No.: 00066
Sequential File No.: 00452 File Date: 12/06/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0520

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:53S		
Control 1 EC	0.097%	09:53S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:53S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54S		
Control 2 EC	0.098%	09:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56S		
Control 3 EC	0.099%	09:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		

All tests within acceptable tolerance.

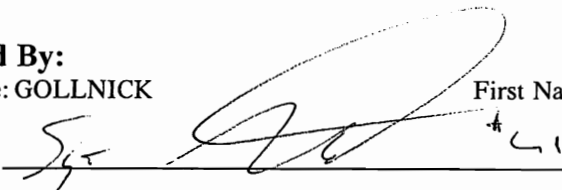
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: GOLLNICK

First Name: MICHAEL

MI: P

Signature: 

Badge No.: 3061

Date: 12/06/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0024
Location: BURLINGTON TOWNSHIP PD
Calibration File No.: 00417 Calib. Date: 08/25/2009 Calib. No.: 00008
Certification File No.: 00418 Cert. Date: 08/25/2009 Cert. No.: 00007
Linearity File No.: 00419 Lin. Date: 08/25/2009 Lin. No.: 00007
Solution File No.: 00456 Soln. Date: 12/30/2009 Soln. No.: 00067
Sequential File No.: 00456 File Date: 12/30/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0166
Control Solution %: 0.100% Expires: 06/09/2010
Solution Control Lot: 08F053 Bottle No.: 0525

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:59S		
Control 1 EC	0.100%	00:00S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:00S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:01S		
Control 2 EC	0.099%	00:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:02S		
Control 3 EC	0.099%	00:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:04S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULLIVAN

First Name: JAMES

MI: B

Signature: 

Badge No.: 70

Date: 12/31/2009