

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: PENNSVILLE P.D.
Calibration File No.: 00295
Certification File No.: 00296
Linearity File No.: 00297
Solution File No.: 00310
Sequential File No.: 00310

Serial No.: ARTN-0044

Calib. Date: 01/30/2009 **Calib. No.:** 00009
Cert. Date: 01/30/2009 **Cert. No.:** 00006
Lin. Date: 01/30/2009 **Lin. No.:** 00006
Soln. Date: 03/25/2009 **Soln. No.:** 00070
File Date: 03/25/2009

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 08A049

Model No.: CU-34

Serial No.: DDUM S3-0239
Expires: 01/09/2010
Bottle No.: 0536

Function	Result	Time	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:37S	10:37 D H.u.	
Control 1 EC	0.102%	09:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38S		
Control 2 EC	0.100%	09:39S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40S		
Control 3 EC	0.100%	09:40S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	09:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41S	10:41 D H.u.	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

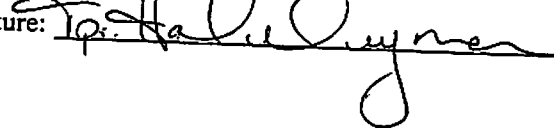
Temperature Probe Serial Number: DDWAP2-063 H.u.

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature:  #6289

Badge No.: 6289

Date: 03/25/2009



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 02/08/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08A049

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1220 to 0.1225 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 9, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 16th day of April, 2008.

Linda L. DeSantis
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009

