

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01981	Calib. Date: 01/31/2011
Certification File No.:	01982	Calib. No.: 00020
Linearity File No.:	01983	Cert. Date: 01/31/2011
Solution File No.:	02015	Cert. No.: 00013
Sequential File No.:	02015	Lin. Date: 01/31/2011
		Lin. No.: 00013
		Soln. Date: 03/11/2011
		Soln. No.: 00204
		File Date: 03/11/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1338

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:50S		
Control 1 EC	0.102%	07:51S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:52S		
Control 2 EC	0.099%	07:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:53S		
Control 3 EC	0.100%	07:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____



Badge No.: 5432

Date: 03/11/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01981	Calib. Date: 01/31/2011
Certification File No.:	01982	Calib. No.: 00020
Linearity File No.:	01983	Cert. Date: 01/31/2011
Solution File No.:	02002	Cert. No.: 00013
Sequential File No.:	02002	Lin. Date: 01/31/2011
		Lin. No.: 00013
		Soln. Date: 02/20/2011
		Soln. No.: 00203
		File Date: 02/20/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1332

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:40S		
Control 1 EC	0.100%	05:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:42S		
Control 2 EC	0.097%	05:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:43S		
Control 3 EC	0.097%	05:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:44S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BROWNE

First Name: MATTHEW

MI: S

Signature: _____

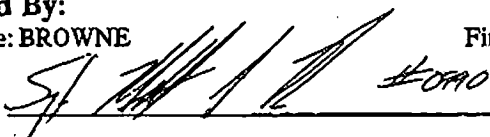

Badge No.: 0990

Date: 02/20/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01843	Calib. Date: 09/14/2010
Certification File No.:	01844	Calib. No.: 00019
Linearity File No.:	01845	Cert. Date: 09/14/2010
Solution File No.:	01954	Cert. No.: 00012
Sequential File No.:	01954	Lin. Date: 09/14/2010
		Lin. No.: 00012
		Soln. Date: 01/06/2011
		Soln. No.: 00199
		File Date: 01/06/2011

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWC S3-0103
Control Solution %:	0.100%		Expires: 03/10/2012
Solution Control Lot:	10C077		Bottle No.: 1333

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:50S		
Control 1 EC	0.104%	14:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	14:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:51S		
Control 2 EC	0.101%	14:52S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	14:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:52S		
Control 3 EC	0.102%	14:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	14:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

Baron McCoy 5432

Badge No.: 5432

Date: 01/06/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01843	Calib. Date: 09/14/2010
Certification File No.:	01844	Calib. No.: 00019
Linearity File No.:	01845	Cert. Date: 09/14/2010
Solution File No.:	01926	Cert. No.: 00012
Sequential File No.:	01926	Lin. Date: 09/14/2010
		Lin. No.: 00012
		Soln. Date: 12/01/2010
		Soln. No.: 00197
		File Date: 12/01/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWC S3-0103
Control Solution %: 0.100%		Expires: 03/10/2012
Solution Control Lot: 10C077		Bottle No.: 1330

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:34S		
Control 1 EC	0.103%	11:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	11:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:35S		
Control 2 EC	0.102%	11:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:37S		
Control 3 EC	0.102%	11:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

R. B. McCoy 5432

Badge No.: 5432

Date: 12/01/2010

Calibrating Unit


New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	Calib. No.: 00019
Calibration File No.:	01843	Cert. No.: 00012
Certification File No.:	01844	Lin. No.: 00012
Linearity File No.:	01845	Soln. No.: 00196
Solution File No.:	01908	
Sequential File No.:	01908	
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	10C077	Expires: 03/10/2012
		Bottle No.: 1329

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:10S		*** TEST PASSED ***
Control 1 EC	0.103%	15:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:11S	34.0°C	
Ambient Air Blank	0.000%	15:11S		*** TEST PASSED ***
Control 2 EC	0.101%	15:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	15:12S	34.0°C	
Ambient Air Blank	0.000%	15:13S		*** TEST PASSED ***
Control 3 EC	0.102%	15:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	15:13S	34.0°C	
Ambient Air Blank	0.000%	15:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:		
Last Name: MCCOY	First Name: BARON	MI: A
Signature: 	Badge No.: 5432	Date: 11/12/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: VINELAND CITY P.D.
Calibration File No.: 01843
Certification File No.: 01844
Linearity File No.: 01845
Solution File No.: 01896
Sequential File No.: 01896

Calib. Date: 09/14/2010
Cert. Date: 09/14/2010
Lin. Date: 09/14/2010
Soln. Date: 10/30/2010
File Date: 10/30/2010

Serial No.: ARWA-0185

Calib. No.: 00019
Cert. No.: 00012
Lin. No.: 00012
Soln. No.: 00195

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 10C077

Model No.: CU-34

Serial No.: DDWC S3-0103
Expires: 03/10/2012
Bottle No.: 1328

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:30D		
Control 1 EC	0.101%	15:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	15:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32D		
Control 2 EC	0.099%	15:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:33D		
Control 3 EC	0.100%	15:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

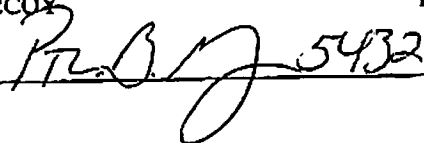

Badge No.: 5432

Date: 10/30/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01843	Calib. Date: 09/14/2010
Certification File No.:	01844	Calib. No.: 00019
Linearity File No.:	01845	Cert. Date: 09/14/2010
Solution File No.:	01859	Cert. No.: 00012
Sequential File No.:	01859	Lin. Date: 09/14/2010
		Lin. No.: 00012
		Soln. Date: 10/01/2010
		Soln. No.: 00191
		File Date: 10/01/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0144

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:57D		
Control 1 EC	0.102%	11:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58D		
Control 2 EC	0.101%	11:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59D		
Control 3 EC	0.101%	12:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

PRB.Mj 5432

Badge No.: 5432

Date: 10/01/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01843	Calib. Date: 09/14/2010
Certification File No.:	01844	Cert. No.: 00019
Linearity File No.:	01845	Cert. Date: 09/14/2010
Solution File No.:	01851	Lin. No.: 00012
Sequential File No.:	01851	Soln. Date: 09/23/2010
		Soln. No.: 00190
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063-	Expires: 02/02/2011
		Bottle No.: 0149

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:00D		
Control 1 EC	0.102%	11:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	11:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01D		
Control 2 EC	0.101%	11:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02D		
Control 3 EC	0.101%	11:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	11:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

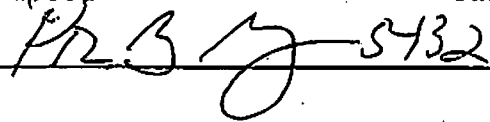

Badge No.: 5432

Date: 09/23/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01786	Cert. No.: 00011
Sequential File No.:	01786	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 08/02/2010
		Soln. No.: 00185
		File Date: 08/02/2010

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWC S3-0103
Control Solution %:	0.100%		Expires: 02/02/2011
Solution Control Lot:	09B063		Bottle No.: 0147

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:43D		
Control 1 EC	0.099%	14:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:44D		
Control 2 EC	0.099%	14:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:45D		
Control 3 EC	0.099%	14:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

R. B. G. 5432

Badge No.: 5432

Date: 08/02/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01776	Cert. No.: 00011
Sequential File No.:	01776	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 07/25/2010
		Soln. No.: 00184
		File Date: 07/25/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0146

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:21D		
Control 1 EC	0.097%	00:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	00:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:22D		
Control 2 EC	0.097%	00:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:23D		
Control 3 EC	0.098%	00:24D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BROWNE

First Name: MATTHEW

MI: S

Signature: _____



Badge No.: 0990

Date: 07/25/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01758	Cert. No.: 00011
Sequential File No.:	01758	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 07/10/2010
		Soln. No.: 00183
		File Date: 07/10/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0131

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:50D		
Control 1 EC	0.099%	03:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:51D		
Control 2 EC	0.099%	03:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:53D		
Control 3 EC	0.098%	03:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSF) Chief Forensic Scientist.


Changed By:

Last Name: BROWNE

First Name: MATTHEW

MI: S

Signature: _____



Badge No.: 0990

Date: 07/10/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01742	Lin. Date: 03/29/2010
Sequential File No.:	01742	Lin. No.: 00011
		Soln. Date: 06/28/2010
		Soln. No.: 00182
		File Date: 06/28/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0141

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:28D		
Control 1 EC	0.101%	22:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:29D		
Control 2 EC	0.100%	22:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:31D		
Control 3 EC	0.100%	22:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	22:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DARRIGO

First Name: PETER

MI: -

Signature: _____

Peter Darrigo # 2173

Badge No.: 2173

Date: 06/28/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01719	Cert. No.: 00011
Sequential File No.:	01719	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 05/30/2010
		Soln. No.: 00181
		File Date: 05/30/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0142

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:11D		
Control 1 EC	0.101%	12:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:13D		
Control 2 EC	0.099%	12:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:14D		
Control 3 EC	0.100%	12:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCANN

First Name: JOHN

MI: J

Signature: _____



Badge No.: 5417

Date: 05/30/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01696	Cert. No.: 00011
Sequential File No.:	01696	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 05/12/2010
		Soln. No.: 00180
		File Date: 05/12/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0128

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:07D		
Control 1 EC	0.099%	13:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:09D		
Control 2 EC	0.099%	13:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:10D		
Control 3 EC	0.099%	13:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature:  5432

Badge No.: 5432

Date: 05/12/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0185
Location:	VINELAND CITY P.D.	Calib. No.:	00018
Calibration File No.:	01641	Cert. No.:	00011
Certification File No.:	01642	Lin. No.:	00011
Linearity File No.:	01643	Soln. No.:	00179
Solution File No.:	01683	Calib. Date:	03/29/2010
Sequential File No.:	01683	Cert. Date:	03/29/2010
		Lin. Date:	03/29/2010
		Soln. Date:	05/02/2010
		File Date:	05/02/2010

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWC S3-0103
Control Solution %:	0.100%			Expires:	02/02/2011
Solution Control Lot:	09B063			Bottle No.:	0139

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:34D		
Control 1 EC	0.101%	00:35D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:36D		
Control 2 EC	0.100%	00:36D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:37D		
Control 3 EC	0.100%	00:37D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	00:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:38D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TESORONI

First Name: DAVID

MI: NA

Signature:



Badge No.: 8329

Date: 05/02/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01677	Cert. No.: 00011
Sequential File No.:	01677	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 04/25/2010
		Soln. No.: 00177
		File Date: 04/25/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0135

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:38D		
Control 1 EC	0.100%	02:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:39D		
Control 2 EC	0.098%	02:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:41D		
Control 3 EC	0.098%	02:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TESORONI

First Name: DAVID

MI: -

Signature: 

Badge No.: 8329

Date: 04/25/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01662	Cert. No.: 00011
Sequential File No.:	01662	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 04/18/2010
		Soln. No.: 00176
		File Date: 04/18/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0126

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:43D		
Control 1 EC	0.098%	09:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		
Control 2 EC	0.097%	09:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		
Control 3 EC	0.098%	09:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SOLAZZO

First Name: VINCENT

MI: P

Signature: _____



Badge No.: 8085

Date: 04/18/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01641	Calib. Date: 03/29/2010
Certification File No.:	01642	Calib. No.: 00018
Linearity File No.:	01643	Cert. Date: 03/29/2010
Solution File No.:	01644	Cert. No.: 00011
Sequential File No.:	01644	Lin. Date: 03/29/2010
		Lin. No.: 00011
		Soln. Date: 03/29/2010
		Soln. No.: 00175
		File Date: 03/29/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWC S3-0102
Control Solution %: 0.100%		Expires: 02/02/2011
Solution Control Lot: 09B063		Bottle No.: 0134

Function	Result	Time	Temperature	Comment(s) or Error(s)
	%BAC	HH:MM	Simulator (°C)	
Ambient Air Blank	0.000%	15:30S	16:30D H ₂ O.	
Control 1 EC	0.101%	15:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:31S		
Control 2 EC	0.099%	15:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:32S		
Control 3 EC	0.100%	15:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:33S	16:33D H ₂ O.	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUNPZ-331 H₂O.

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature: 

Badge No.: 6289

Date: 03/29/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0185
Location:	VINELAND CITY P.D.		
Calibration File No.:	01469	Calib. Date:	10/19/2009
Certification File No.:	01470	Calib. No.:	00017
Linearity File No.:	01471	Cert. Date:	10/19/2009
Solution File No.:	01633	Cert. No.:	00010
Sequential File No.:	01633	Lin. Date:	10/19/2009
		Lin. No.:	00010
		Soln. Date:	03/26/2010
		Soln. No.:	00174
		File Date:	03/26/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWC S3-0103
Solution Control Lot:	09B063	Expires:	02/02/2011
		Bottle No.:	0140

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:45S		
Control 1 EC	0.104%	10:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	10:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47S		
Control 2 EC	0.103%	10:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	10:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48S		
Control 3 EC	0.103%	10:48S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	10:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

Handwritten signature: P. B. Baron

5432

Badge No.: 5432

Date: 03/26/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01469	Calib. Date: 10/19/2009
Certification File No.:	01470	Calib. No.: 00017
Linearity File No.:	01471	Cert. Date: 10/19/2009
Solution File No.:	01606	Cert. No.: 00010
Sequential File No.:	01606	Lin. Date: 10/19/2009
		Lin. No.: 00010
		Soln. Date: 02/27/2010
		Soln. No.: 00173
		File Date: 02/27/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC 83-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0132

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:56S		
Control 1 EC	0.103%	17:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	17:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:57S		
Control 2 EC	0.101%	17:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	17:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:58S		
Control 3 EC	0.103%	17:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	17:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DEMARY

First Name: FREDRICK

MI: S

Signature: _____

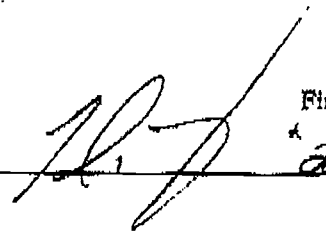

* 2291

Badge No.: 2291

Date: 02/27/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01469	Calib. Date: 10/19/2009
Certification File No.:	01470	Calib. No.: 00017
Linearity File No.:	01471	Cert. Date: 10/19/2009
Solution File No.:	01581	Cert. No.: 00010
Sequential File No.:	01581	Lin. Date: 10/19/2009
		Lin. No.: 00010
		Soln. Date: 02/02/2010
		Soln. No.: 00171
		File Date: 02/02/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0721

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:28S		
Control 1 EC	0.104%	09:29S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.105%	09:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30S		
Control 2 EC	0.102%	09:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 3 EC	0.103%	09:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	09:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TESORONI

First Name: DAVID

MI:

Signature:

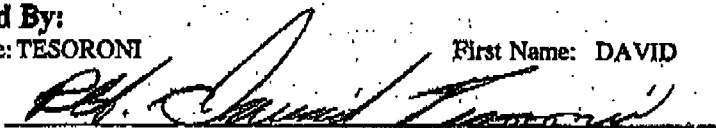

Badge No.: 8329

Date: 02/02/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01469	Calib. Date: 10/19/2009
Certification File No.:	01470	Calib. No.: 00017
Linearity File No.:	01471	Cert. Date: 10/19/2009
Solution File No.:	01562	Cert. No.: 00010
Sequential File No.:	01562	Lin. Date: 10/19/2009
		Lin. No.: 00010
		Soln. Date: 01/16/2010
		Soln. No.: 00170
		File Date: 01/16/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0722

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:07S		
Control 1 EC	0.103%	08:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	08:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08S		
Control 2 EC	0.103%	08:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	08:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		
Control 3 EC	0.103%	08:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	08:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

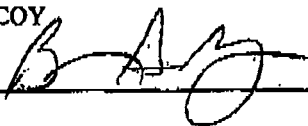

Badge No.: 5432

Date: 01/16/2010