

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01469	Calib. Date: 10/19/2009
Certification File No.:	01470	Calib. No.: 00017
Linearity File No.:	01471	Cert. Date: 10/19/2009
Solution File No.:	01541	Cert. No.: 00010
Sequential File No.:	01541	Lin. Date: 10/19/2009
		Lin. No.: 00010
		Soln. Date: 12/26/2009
		Soln. No.: 00169
		File Date: 12/26/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09B063	Expires: 02/02/2011
		Bottle No.: 0137

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:15S		
Control 1 EC	0.103%	01:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	01:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:16S		
Control 2 EC	0.102%	01:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	01:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:18S		
Control 3 EC	0.103%	01:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	01:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCANN

First Name: JOHN

MI: J

Signature: 

Badge No.: 5417

Date: 12/26/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01469	Calib. Date: 10/19/2009
Certification File No.:	01470	Calib. No.: 00017
Linearity File No.:	01471	Cert. Date: 10/19/2009
Solution File No.:	01513	Cert. No.: 00010
Sequential File No.:	01513	Lin. Date: 10/19/2009
		Lin. No.: 00010
		Soln. Date: 12/01/2009
		Soln. No.: 00167
		File Date: 12/01/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0711

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:02S		
Control 1 EC	0.100%	15:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03S		
Control 2 EC	0.100%	15:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:04S		
Control 3 EC	0.100%	15:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

PTL. B.M. 5432

Badge No.: 5432

Date: 12/01/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0185
Location:	VINELAND CITY P.D.		
Calibration File No.:	01469	Calib. Date:	10/19/2009
Certification File No.:	01470	Cert. Date:	10/19/2009
Linearity File No.:	01471	Lin. Date:	10/19/2009
Solution File No.:	01487	Soln. Date:	11/07/2009
Sequential File No.:	01487	File Date:	11/07/2009

Calib. No.:	00017
Cert. No.:	00010
Lin. No.:	00010
Soln. No.:	00165

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWC S3-0103
Control Solution %:	0.100%			Expires:	01/15/2011
Solution Control Lot:	09A062			Bottle No.:	0723

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:58S		
Control 1 EC	0.103%	05:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	05:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:59S		
Control 2 EC	0.102%	06:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	06:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:00S		
Control 3 EC	0.102%	06:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TESORONI

First Name: DAVID

MI: N.

Signature: 

Badge No.: 8329

Date: 11/07/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: VINELAND CITY P.D.
Calibration File No.: 01275
Certification File No.: 01276
Linearity File No.: 01277
Solution File No.: 01462
Sequential File No.: 01462

Serial No.: ARWA-0185

Calib. Date: 05/05/2009
Cert. Date: 05/05/2009
Lin. Date: 05/05/2009
Soln. Date: 10/05/2009
File Date: 10/05/2009

Calib. No.: 00016
Cert. No.: 00009
Lin. No.: 00009
Soln. No.: 00162

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 09B063

Model No.: CU-34

Serial No.: DDWC S3-0103
Expires: 02/02/2011
Bottle No.: 0129

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:56D		
Control 1 EC	0.100%	08:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57D		
Control 2 EC	0.099%	08:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:58D		
Control 3 EC	0.099%	08:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:
Last Name: SOLAZZO

First Name: VINCENT

MI: P

Signature: Sgt. V. S.

Badge No.: 8085

Date: 10/05/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0185
Location:	VINELAND CITY P.D.		
Calibration File No.:	01275	Calib. Date:	05/05/2009
Certification File No.:	01276	Cert. Date:	05/05/2009
Linearity File No.:	01277	Lin. Date:	05/05/2009
Solution File No.:	01427	Soln. Date:	09/10/2009
Sequential File No.:	01427	File Date:	09/10/2009

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDWC S3-0103
Control Solution %:	0.100%			Expires:	01/15/2011
Solution Control Lot:	09A062			Bottle No.:	0706

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:01D		
Control 1 EC	0.100%	08:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 2 EC	0.100%	08:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:04D		
Control 3 EC	0.099%	08:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

Baron McCoy

Badge No.: 5432

Date: 09/10/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01275	Calib. Date: 05/05/2009
Certification File No.:	01276	Calib. No.: 00016
Linearity File No.:	01277	Cert. Date: 05/05/2009
Solution File No.:	01411	Cert. No.: 00009
Sequential File No.:	01411	Lin. Date: 05/05/2009
		Lin. No.: 00009
		Soln. Date: 08/26/2009
		Soln. No.: 00159
		File Date: 08/26/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0701

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:29D		
Control 1 EC	0.100%	11:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:30D		
Control 2 EC	0.099%	11:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 3 EC	0.099%	11:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

R. B. M. 5432

Badge No.: 5432

Date: 08/26/2009

Calibrating Unit New Standard Solution Report

6

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01275	Callb. Date: 05/05/2009
Certification File No.:	01276	Callb. No.: 00016
Linearity File No.:	01277	Cert. Date: 05/05/2009
Solution File No.:	01403	Cert. No.: 00009
Sequential File No.:	01403	Lin. Date: 05/05/2009
		Lin. No.: 00009
		Soln. Date: 08/21/2009
		Soln. No.: 00158
		File Date: 08/21/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0720

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:42D		
Control 1 EC	0.098%	09:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43D		
Control 2 EC	0.098%	09:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		
Control 3 EC	0.099%	09:45D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

RBG-5432

Badge No.: 5432

Date: 08/21/2009

Calibrating Unit New Standard Solution Report

Equipment: Alcotest 7110 MKIII-C
 Location: VINELAND CITY P.D.
 Calibration File No.: 01275
 Certification File No.: 01276
 Linearity File No.: 01277
 Solution File No.: 01368
 Sequential File No.: 01368

Calib. Date: 05/05/2009
 Cert. Date: 05/05/2009
 Lin. Date: 05/05/2009
 Soln. Date: 07/26/2009
 File Date: 07/26/2009

Serial No.: ARWA-0185

Calib. No.: 00016
 Cert. No.: 00009
 Lin. No.: 00009
 Soln. No.: 00156

Calibrating Unit: WET
 Control Solution %: 0.100%
 Solution Control Lot: 09B063

Model No.: CU-34

Serial No.: DDWC 33-0103
 Expires: 02/02/2011
 Bottle No.: 0130

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:18D		
Control 1 EC	0.100%	11:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		
Control 2 EC	0.099%	11:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21D		
Control 3 EC	0.099%	11:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TESORONI

First Name: DAVID

MI: -

Signature: 

Badge No.: 8329

Date: 07/26/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: VINELAND CITY P.D.
Calibration File No.: 01275
Certification File No.: 01276
Linearity File No.: 01277
Solution File No.: 01333
Sequential File No.: 01333

Serial No.: ARWA-0185
Calib. No.: 00016
Cert. No.: 00009
Lin. No.: 00009
Soln. No.: 00154

Calib. Date: 05/05/2009
Cert. Date: 05/05/2009
Lin. Date: 05/05/2009
Soln. Date: 06/27/2009
File Date: 06/27/2009

Calibrating Unit: WBT
Control Solution %: 0.100%
Solution Control Lot: 08B050

Model No.: CU-34

Serial No.: DDWC S3-0103
Expires: 02/13/2010
Bottle No.: 1175

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:43D		
Control 1 EC	0.100%	13:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:44D		
Control 2 EC	0.099%	13:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:46D		
Control 3 EC	0.100%	13:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:
Last Name: SOLAZZO

First Name: VINCENT

MI P

Signature: _____



Badge No.: 8085
Date: 06/27/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01275	Calib. Date: 05/05/2009
Certification File No.:	01276	Calb. No.: 00016
Linearity File No.:	01277	Cert. No.: 00009
Solution File No.:	01319	Lin. Date: 05/05/2009
Sequential File No.:	01319	Lin. No.: 00009
		Soln. Date: 06/09/2009
		Soln. No.: 00153
		File Date: 06/09/2009

Calibrating Unit:	WBT	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0103
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0709

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:28D		
Control 1 EC	0.102%	12:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:29D		
Control 2 EC	0.101%	12:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 3 EC	0.101%	12:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUNP2-323ams

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: TPR. I. Adam T. Stanks #5403

Badge No.: 5403

Date: 06/09/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01275	Calib. Date: 05/05/2009
Certification File No.:	01276	Calib. No.: 00016
Linearity File No.:	01277	Cert. Date: 05/05/2009
Solution File No.:	01278	Cert. No.: 00009
Sequential File No.:	01278	Lin. Date: 05/05/2009
		Lin. No.: 00009
		Soln. Date: 05/05/2009
		Soln. No.: 00145
		File Date: 05/05/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWC S3-0103
Control Solution %:	0.100%		Expires: 02/13/2010
Solution Control Lot:	08B050		Bottle No.: 1173

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:50D		
Control 1 EC	0.100%	11:50D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51D		
Control 2 EC	0.100%	11:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52D		
Control 3 EC	0.100%	11:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUNP2-323 *ams*

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: TPR. E Adam N. Stanks #5403

Badge No.: 5403

Date: 05/05/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01242	Cert. No.: 00008
Sequential File No.:	01242	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 04/12/2009
		Soln. No.: 00142
		File Date: 04/12/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWC S3-0102
Control Solution %: 0.100%		Expires: 02/13/2010
Solution Control Lot: 08B050		Bottle No.: 1160

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:37D		
Control 1 EC	0.101%	09:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:39D		
Control 2 EC	0.100%	09:39D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40D		
Control 3 EC	0.101%	09:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOLAZZO

First Name: VINCENT

MI: P

Signature: _____

Badge No.: 8085

Date: 04/12/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01223	Cert. No.: 00008
Sequential File No.:	01223	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 03/26/2009
		Soln. No.: 00141
		File Date: 03/26/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 1156

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:07S		
Control 1 EC	0.100%	11:08S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08S		
Control 2 EC	0.100%	11:09S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:09S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10S		
Control 3 EC	0.100%	11:10S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:10S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

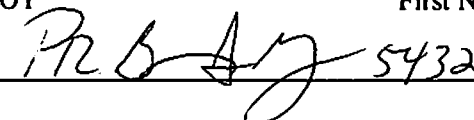

Badge No.: 5432

Date: 03/26/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01205	Cert. No.: 00008
Sequential File No.:	01205	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 03/08/2009
		Soln. No.: 00139
		File Date: 03/08/2009

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 1166

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:47S		
Control 1 EC	0.099%	18:48S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:48S		
Control 2 EC	0.100%	18:49S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:49S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:50S		
Control 3 EC	0.100%	18:50S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SOLAZZO

First Name: VINCENET

Mf: P

Signature: _____



Badge No.: 8085

Date: 03/08/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01179	Cert. No.: 00008
Sequential File No.:	01179	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 02/20/2009
		Soln. No.: 00138
		File Date: 02/20/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWC S3-0102
Control Solution %:	0.100%		Expires: 02/13/2010
Solution Control Lot:	08B050		Bottle No.: 1168

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:55S		
Control 1 EC	0.099%	08:56S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56S		
Control 2 EC	0.100%	08:57S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:58S		
Control 3 EC	0.100%	08:58S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:58S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOLAZZO

First Name: VINCENT

MI: P

Signature: _____

Sgt. V. S2

Badge No.: 8085

Date: 02/20/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0185
Location: VINELAND CITY P.D.
Calibration File No.: 01098 **Calib. Date:** 12/11/2008 **Calib. No.:** 00015
Certification File No.: 01099 **Cert. Date:** 12/11/2008 **Cert. No.:** 00008
Linearity File No.: 01100 **Lin. Date:** 12/11/2008 **Lin. No.:** 00008
Solution File No.: 01160 **Soln. Date:** 02/02/2009 **Soln. No.:** 00137
Sequential File No.: 01160 **File Date:** 02/02/2009

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWC S3-0102
Control Solution %: 0.100% **Expires:** 02/13/2010
Solution Control Lot: 08B050 **Bottle No.:** 1163

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:48S		
Control 1 EC	0.101%	12:48S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:49S		
Control 2 EC	0.101%	12:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:50S		
Control 3 EC	0.101%	12:51S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: FRB. J. 5432

Badge No.: 5432

Date: 02/02/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01146	Cert. No.: 00008
Sequential File No.:	01146	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 01/25/2009
		Soln. No.: 00136
		File Date: 01/25/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 1165

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:16S		
Control 1 EC	0.103%	02:17S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	02:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:17S		
Control 2 EC	0.102%	02:18S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:19S		
Control 3 EC	0.102%	02:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	02:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCANN

First Name: JOHN

MI: J

Signature: Sgt - John McCann # 5417

Badge No.: 5417

Date: 01/25/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01128	Cert. No.: 00008
Sequential File No.:	01128	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 01/06/2009
		Soln. No.: 00135
		File Date: 01/06/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWC S3-0102
Control Solution %: 0.100%		Expires: 02/13/2010
Solution Control Lot: 08B050		Bottle No.: 1170

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:56S		
Control 1 EC	0.101%	10:57S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:57S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:58S		
Control 2 EC	0.101%	10:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	10:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59S		
Control 3 EC	0.101%	10:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOLAZZO

First Name: VINCENT

MI: P

Signature: _____

Sgt. V. S

Badge No.: 8085

Date: 01/06/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0185
Location: VINELAND CITY P.D.
Calibration File No.: 01098 **Calib. Date:** 12/11/2008 **Calib. No.:** 00015
Certification File No.: 01099 **Cert. Date:** 12/11/2008 **Cert. No.:** 00008
Linearity File No.: 01100 **Lin. Date:** 12/11/2008 **Lin. No.:** 00008
Solution File No.: 01120 **Soln. Date:** 12/31/2008 **Soln. No.:** 00134
Sequential File No.: 01120 **File Date:** 12/31/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWC S3-0102
Control Solution %: 0.100% **Expires:** 02/13/2010
Solution Control Lot: 08B050 **Bottle No.:** 1160

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:32S		
Control 1 EC	0.100%	21:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	21:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:33S		
Control 2 EC	0.101%	21:34S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:34S		
Control 3 EC	0.101%	21:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: VAI

First Name: DAVID

MI: A

Signature: _____

Badge No.: 8645

Date: 12/31/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01098	Calib. Date: 12/11/2008
Certification File No.:	01099	Calib. No.: 00015
Linearity File No.:	01100	Cert. Date: 12/11/2008
Solution File No.:	01101	Cert. No.: 00008
Sequential File No.:	01101	Lin. Date: 12/11/2008
		Lin. No.: 00008
		Soln. Date: 12/11/2008
		Soln. No.: 00133
		File Date: 12/11/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 1174

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:30S		
Control 1 EC	0.100%	17:31S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	17:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:31S		
Control 2 EC	0.101%	17:32S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:32S		
Control 3 EC	0.101%	17:33S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	17:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUNP2-331₂₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tpr. II J. Dellanoce # 6027

Badge No.: 6027

Date: 12/11/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01093	Cert. No.: 00007
Sequential File No.:	01093	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 11/21/2008
		Soln. No.: 00130
		File Date: 11/21/2008

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 1151

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:58S		
Control 1 EC	0.098%	07:58S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	07:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:59S		
Control 2 EC	0.096%	07:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	07:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00S		
Control 3 EC	0.097%	08:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:01S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

R. B. A. J. 5432

Badge No.: 5432

Date: 11/21/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0185
Location: VINELAND CITY P.D.
Calibration File No.: 01006 **Calib. Date:** 08/28/2008 **Calib. No.:** 00012
Certification File No.: 01007 **Cert. Date:** 08/28/2008 **Cert. No.:** 00007
Linearity File No.: 01008 **Lin. Date:** 08/28/2008 **Lin. No.:** 00007
Solution File No.: 01086 **Soln. Date:** 11/13/2008 **Soln. No.:** 00128
Sequential File No.: 01086 **File Date:** 11/13/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWC S3-0102
Control Solution %: 0.100% **Expires:** 02/13/2010
Solution Control Lot: 08B050 **Bottle No.:** 1154

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:15S		
Control 1 EC	0.100%	23:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:16S		
Control 2 EC	0.099%	23:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:18S		
Control 3 EC	0.098%	23:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MCCOY

First Name: BARON

MI: A

Signature: _____

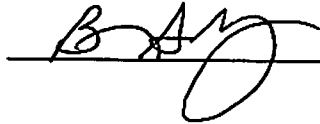

Badge No.: 5432

Date: 11/13/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0185
Location: VINELAND CITY P.D.
Calibration File No.: 01006 **Calib. Date:** 08/28/2008 **Calib. No.:** 00012
Certification File No.: 01007 **Cert. Date:** 08/28/2008 **Cert. No.:** 00007
Linearity File No.: 01008 **Lin. Date:** 08/28/2008 **Lin. No.:** 00007
Solution File No.: 01075 **Soln. Date:** 11/06/2008 **Soln. No.:** 00127
Sequential File No.: 01075 **File Date:** 11/06/2008

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWC S3-0102
Control Solution %: 0.100% **Expires:** 02/13/2010
Solution Control Lot: 08B050 **Bottle No.:** 1152

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:35S		
Control 1 EC	0.096%	04:36S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	04:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:36S		
Control 2 EC	0.096%	04:37S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	04:37S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:38S		
Control 3 EC	0.096%	04:38S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	04:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:39S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature: _____

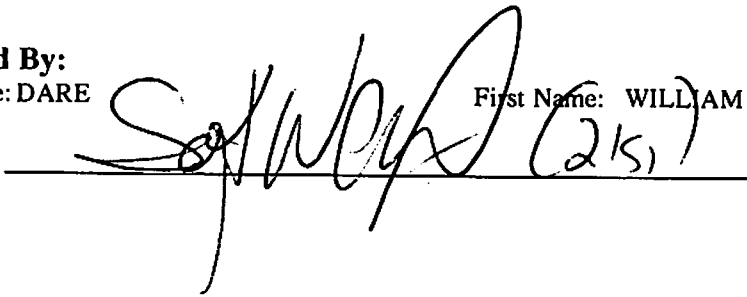

Badge No.: 2151

Date: 11/06/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0185
Location:	VINELAND CITY P.D.		
Calibration File No.:	01006	Calib. Date:	08/28/2008
Certification File No.:	01007	Cert. No.:	00012
Linearity File No.:	01008	Cert. Date:	08/28/2008
Solution File No.:	01072	Lin. Date:	08/28/2008
Sequential File No.:	01072	Lin. No.:	00007
		Soln. Date:	11/03/2008
		Soln. No.:	00126
		File Date:	11/03/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWC S3-0102
Solution Control Lot:	08B050	Expires:	02/13/2010
		Bottle No.:	1153

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:14S		
Control 1 EC	0.099%	09:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15S		
Control 2 EC	0.098%	09:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17S		
Control 3 EC	0.098%	09:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: VAI

First Name: DAVID

MI: A

Signature: _____

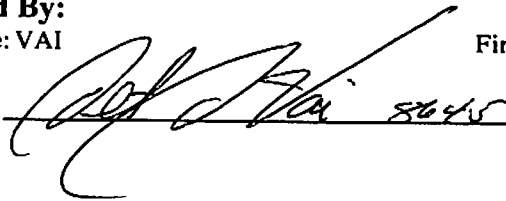

Badge No.: 8645

Date: 11/03/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01059	Cert. No.: 00007
Sequential File No.:	01059	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 10/26/2008
		Soln. No.: 00125
		File Date: 10/26/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	07G047	Expires: 07/23/2009
		Bottle No.: 1129

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:34S		
Control 1 EC	0.099%	09:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:35S		
Control 2 EC	0.097%	09:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:37S		
Control 3 EC	0.097%	09:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature: _____

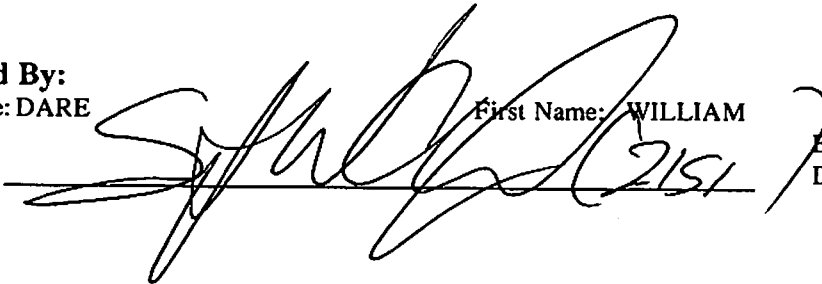

Badge No.: 2151

Date: 10/26/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01052	Cert. No.: 00007
Sequential File No.:	01052	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 10/18/2008
		Soln. No.: 00124
		File Date: 10/18/2008

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWC S3-0102
Control Solution %: 0.100%		Expires: 07/23/2009
Solution Control Lot: 07G047		Bottle No.: 1150

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:17D		
Control 1 EC	0.100%	12:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18D		
Control 2 EC	0.097%	12:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	12:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		
Control 3 EC	0.097%	12:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature:

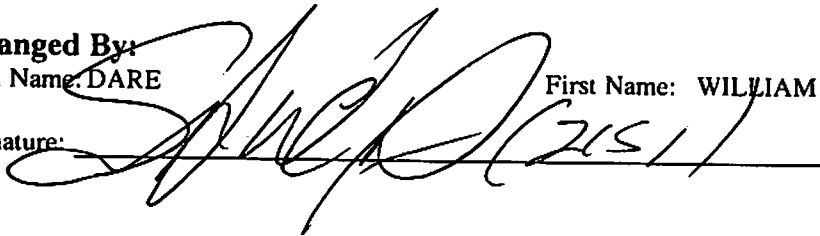

Badge No.: 2151

Date: 10/18/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01044	Cert. No.: 00007
Sequential File No.:	01044	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 10/05/2008
		Soln. No.: 00123
		File Date: 10/05/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	07G047	Expires: 07/23/2009
		Bottle No.: 1134

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:19D		
Control 1 EC	0.098%	01:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:20D		
Control 2 EC	0.097%	01:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:22D		
Control 3 EC	0.097%	01:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature:

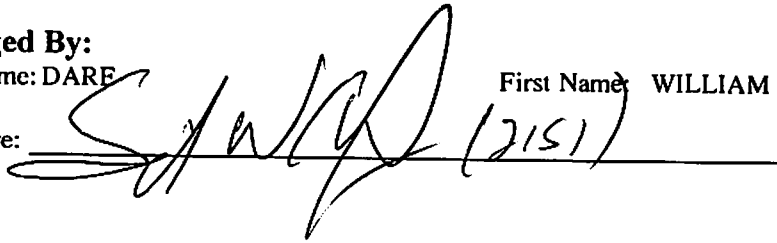

Badge No.: 2151

Date: 10/05/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01037	Cert. No.: 00007
Sequential File No.:	01037	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 09/22/2008
		Soln. No.: 00122
		File Date: 09/22/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	07G047	Expires: 07/23/2009
		Bottle No.: 1145

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:11D		
Control 1 EC	0.099%	09:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:12D		
Control 2 EC	0.098%	09:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		
Control 3 EC	0.098%	09:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature: _____



Badge No.: 2151

Date: 09/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0185
Location:	VINELAND CITY P.D.	
Calibration File No.:	01006	Calib. Date: 08/28/2008
Certification File No.:	01007	Calib. No.: 00012
Linearity File No.:	01008	Cert. Date: 08/28/2008
Solution File No.:	01022	Cert. No.: 00007
Sequential File No.:	01022	Lin. Date: 08/28/2008
		Lin. No.: 00007
		Soln. Date: 09/10/2008
		Soln. No.: 00121
		File Date: 09/10/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWC S3-0102
Solution Control Lot:	07G047	Expires: 07/23/2009
		Bottle No.: 1140

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:15D		
Control 1 EC	0.099%	09:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		
Control 2 EC	0.098%	09:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17D		
Control 3 EC	0.098%	09:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DARE

First Name: WILLIAM

MI: C

Signature: _____

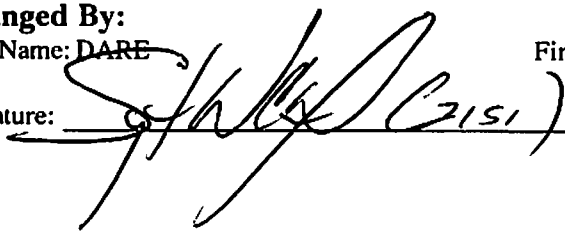

Badge No.: 2151

Date: 09/10/2008