

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00534 Calib. Date: 12/01/2011 Calib. No.: 00016
Certification File No.: 00535 Cert. Date: 12/01/2011 Cert. No.: 00011
Linearity File No.: 00536 Lin. Date: 12/01/2011 Lin. No.: 00011
Solution File No.: 00540 Soln. Date: 12/29/2011 Soln. No.: 00120
Sequential File No.: 00540 File Date: 12/29/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0171

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:46S		
Control 1 EC	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47S		
Control 2 EC	0.098%	09:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49S		
Control 3 EC	0.098%	09:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph Baumgardner #312 12/29/2011

Badge No.: 312

Date: 12/29/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00502	Calib. Date: 07/01/2011
Certification File No.:	00503	Calib. No.: 00015
Linearity File No.:	00504	Cert. Date: 07/01/2011
Solution File No.:	00533	Cert. No.: 00010
Sequential File No.:	00533	Lin. Date: 07/01/2011
		Lin. No.: 00010
		Soln. Date: 11/07/2011
		Soln. No.: 00118
		File Date: 11/07/2011

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	10H081	Expires: 08/04/2012
		Bottle No.: 0172

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:46S		
Control 1 EC	0.101%	14:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:48S		
Control 2 EC	0.101%	14:48S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:49S		
Control 3 EC	0.100%	14:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Sergeant Joseph T. Baumgardner #312 / 11/07/2011

Badge No.: 312

Date: 11/07/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00502	Calib. Date: 07/01/2011
Certification File No.:	00503	Calib. No.: 00015
Linearity File No.:	00504	Cert. Date: 07/01/2011
Solution File No.:	00530	Cert. No.: 00010
Sequential File No.:	00530	Lin. Date: 07/01/2011
		Lin. No.: 00010
		Soln. Date: 10/11/2011
		Soln. No.: 00117
		File Date: 10/11/2011

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	10H081	Expires: 08/04/2012
		Bottle No.: 0162

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:20D		
Control 1 EC	0.100%	03:21D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:21D		
Control 2 EC	0.099%	03:22D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:23D		
Control 3 EC	0.099%	03:23D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Joseph T. Baumgardner #312 10/11/2011

Badge No.: 312

Date: 10/11/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00502 Calib. Date: 07/01/2011 Calib. No.: 00015
Certification File No.: 00503 Cert. Date: 07/01/2011 Cert. No.: 00010
Linearity File No.: 00504 Lin. Date: 07/01/2011 Lin. No.: 00010
Solution File No.: 00528 Soln. Date: 09/12/2011 Soln. No.: 00116
Sequential File No.: 00528 File Date: 09/12/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0153

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:04D		
Control 1 EC	0.099%	21:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:05D		
Control 2 EC	0.099%	21:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:06D		
Control 3 EC	0.099%	21:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 09/12/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00502	Calib. Date: 07/01/2011
Certification File No.:	00503	Calib. No.: 00015
Linearity File No.:	00504	Cert. Date: 07/01/2011
Solution File No.:	00527	Cert. No.: 00010
Sequential File No.:	00527	Lin. Date: 07/01/2011
		Lin. No.: 00010
		Soln. Date: 09/12/2011
		Soln. No.: 00115
		File Date: 09/12/2011

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	10H081	Expires: 08/04/2012
		Bottle No.: 0167

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:31D		
Control 1 EC	-.---%	19:32D	21.6°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	19:32D	21.6°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 09/12/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00502 Calib. Date: 07/01/2011 Calib. No.: 00015
Certification File No.: 00503 Cert. Date: 07/01/2011 Cert. No.: 00010
Linearity File No.: 00504 Lin. Date: 07/01/2011 Lin. No.: 00010
Solution File No.: 00522 Soln. Date: 08/10/2011 Soln. No.: 00114
Sequential File No.: 00522 File Date: 08/10/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0154

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:09D		
Control 1 EC	0.099%	13:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:11D		
Control 2 EC	0.100%	13:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:12D		
Control 3 EC	0.099%	13:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 08/10/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00502 Calib. Date: 07/01/2011 Calib. No.: 00015
Certification File No.: 00503 Cert. Date: 07/01/2011 Cert. No.: 00010
Linearity File No.: 00504 Lin. Date: 07/01/2011 Lin. No.: 00010
Solution File No.: 00515 Soln. Date: 07/15/2011 Soln. No.: 00113
Sequential File No.: 00515 File Date: 07/15/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0175

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:21D		
Control 1 EC	0.099%	06:22D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:23D		
Control 2 EC	0.099%	06:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:24D		
Control 3 EC	0.099%	06:24D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

PHM. JAMES 319

Badge No.: 319

Date: 07/15/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00459 Calib. Date: 01/25/2011 Calib. No.: 00014
Certification File No.: 00460 Cert. Date: 01/25/2011 Cert. No.: 00009
Linearity File No.: 00461 Lin. Date: 01/25/2011 Lin. No.: 00009
Solution File No.: 00500 Soln. Date: 06/26/2011 Soln. No.: 00111
Sequential File No.: 00500 File Date: 06/26/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0168

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:09D		
Control 1 EC	0.097%	08:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		
Control 2 EC	0.097%	08:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11D		
Control 3 EC	0.097%	08:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

James Silva #319

Badge No.: 319

Date: 06/26/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00459	Calib. Date: 01/25/2011
Certification File No.:	00460	Calib. No.: 00014
Linearity File No.:	00461	Cert. Date: 01/25/2011
Solution File No.:	00487	Cert. No.: 00009
Sequential File No.:	00487	Lin. Date: 01/25/2011
		Lin. No.: 00009
		Soln. Date: 06/06/2011
		Soln. No.: 00110
		File Date: 06/06/2011

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	10H081	Expires: 08/04/2012
		Bottle No.: 0163

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:37D		
Control 1 EC	0.099%	08:37D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:38D		
Control 2 EC	0.098%	08:38D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:39D		
Control 3 EC	0.099%	08:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

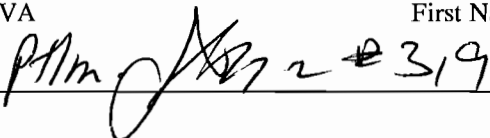

Badge No.: 319

Date: 06/06/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00459 Calib. Date: 01/25/2011 Calib. No.: 00014
Certification File No.: 00460 Cert. Date: 01/25/2011 Cert. No.: 00009
Linearity File No.: 00461 Lin. Date: 01/25/2011 Lin. No.: 00009
Solution File No.: 00479 Soln. Date: 05/09/2011 Soln. No.: 00109
Sequential File No.: 00479 File Date: 05/09/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0159

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:58D		
Control 1 EC	0.099%	20:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	20:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:00D		
Control 2 EC	0.098%	21:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:01D		
Control 3 EC	0.099%	21:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 05/09/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00459	Calib. Date: 01/25/2011
Certification File No.:	00460	Calib. No.: 00014
Linearity File No.:	00461	Cert. Date: 01/25/2011
Solution File No.:	00474	Cert. No.: 00009
Sequential File No.:	00474	Lin. Date: 01/25/2011
		Lin. No.: 00009
		Soln. Date: 04/12/2011
		Soln. No.: 00108
		File Date: 04/12/2011
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	10H081	Expires: 08/04/2012
		Bottle No.: 0169

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:19D		
Control 1 EC	0.099%	11:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21D		
Control 2 EC	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		
Control 3 EC	0.098%	11:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

Badge No.: 319

Date: 04/12/2011

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00459	Calib. Date: 01/25/2011
Certification File No.:	00460	Calib. No.: 00014
Linearity File No.:	00461	Cert. Date: 01/25/2011
Solution File No.:	00473	Cert. No.: 00009
Sequential File No.:	00473	Lin. Date: 01/25/2011
		Lin. No.: 00009
		Soln. Date: 04/12/2011
		Soln. No.: 00107
		File Date: 04/12/2011

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %:	0.100%		Expires: 08/04/2012
Solution Control Lot:	10H081		Bottle No.: 0164

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:05D		
Control 1 EC	-.--%	08:05D	21.9°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.--%	08:05D	21.9°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.--%	--:--		
Control 2 EC	-.--%	--:--	N/A	
Control 2 IR	-.--%	--:--	N/A	
Ambient Air Blank	-.--%	--:--		
Control 3 EC	-.--%	--:--	N/A	
Control 3 IR	-.--%	--:--	N/A	
Ambient Air Blank	-.--%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

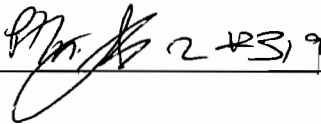

Badge No.: 319

Date: 04/12/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00459 Calib. Date: 01/25/2011 Calib. No.: 00014
Certification File No.: 00460 Cert. Date: 01/25/2011 Cert. No.: 00009
Linearity File No.: 00461 Lin. Date: 01/25/2011 Lin. No.: 00009
Solution File No.: 00470 Soln. Date: 03/19/2011 Soln. No.: 00106
Sequential File No.: 00470 File Date: 03/19/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0155

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:04S		
Control 1 EC	0.099%	09:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05S		
Control 2 EC	0.099%	09:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:07S		
Control 3 EC	0.099%	09:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 3/19/2011

Badge No.: 312

Date: 03/19/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00459 Calib. Date: 01/25/2011 Calib. No.: 00014
Certification File No.: 00460 Cert. Date: 01/25/2011 Cert. No.: 00009
Linearity File No.: 00461 Lin. Date: 01/25/2011 Lin. No.: 00009
Solution File No.: 00465 Soln. Date: 02/20/2011 Soln. No.: 00105
Sequential File No.: 00465 File Date: 02/20/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0170

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:02S		
Control 1 EC	0.099%	08:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03S		
Control 2 EC	0.098%	08:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:05S		
Control 3 EC	0.098%	08:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

Pt/m. [Signature] #319

Badge No.: 319

Date: 02/20/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00433 Calib. Date: 08/13/2010 Calib. No.: 00013
Certification File No.: 00434 Cert. Date: 08/13/2010 Cert. No.: 00008
Linearity File No.: 00435 Lin. Date: 08/13/2010 Lin. No.: 00008
Solution File No.: 00455 Soln. Date: 01/03/2011 Soln. No.: 00103
Sequential File No.: 00455 File Date: 01/03/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 08/04/2012
Solution Control Lot: 10H081 Bottle No.: 0165

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:56S		
Control 1 EC	0.101%	08:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:57S		
Control 2 EC	0.099%	08:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:58S		
Control 3 EC	0.099%	08:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:00S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 01/03/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00433 Calib. Date: 08/13/2010 Calib. No.: 00013
Certification File No.: 00434 Cert. Date: 08/13/2010 Cert. No.: 00008
Linearity File No.: 00435 Lin. Date: 08/13/2010 Lin. No.: 00008
Solution File No.: 00454 Soln. Date: 12/07/2010 Soln. No.: 00102
Sequential File No.: 00454 File Date: 12/07/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0166

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:01S		
Control 1 EC	0.100%	10:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02S		
Control 2 EC	0.099%	10:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		
Control 3 EC	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph Baumgardner #312 12/7/2010

Badge No.: 312

Date: 12/07/2010



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 8/26/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10H081

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1185 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 4, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 9 day of September, 2010.

Handwritten signature of John R. Leaver
Notary
JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00433 Calib. Date: 08/13/2010 Calib. No.: 00013
Certification File No.: 00434 Cert. Date: 08/13/2010 Cert. No.: 00008
Linearity File No.: 00435 Lin. Date: 08/13/2010 Lin. No.: 00008
Solution File No.: 00453 Soln. Date: 11/12/2010 Soln. No.: 00101
Sequential File No.: 00453 File Date: 11/12/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0156

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:13S		
Control 1 EC	0.100%	08:13S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:14S		
Control 2 EC	0.100%	08:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:15S		
Control 3 EC	0.101%	08:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

James Silva #319

Badge No.: 319

Date: 11/12/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00433 Calib. Date: 08/13/2010 Calib. No.: 00013
Certification File No.: 00434 Cert. Date: 08/13/2010 Cert. No.: 00008
Linearity File No.: 00435 Lin. Date: 08/13/2010 Lin. No.: 00008
Solution File No.: 00452 Soln. Date: 10/31/2010 Soln. No.: 00100
Sequential File No.: 00452 File Date: 10/31/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0157

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:38S		
Control 1 EC	0.100%	04:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:39S		
Control 2 EC	0.099%	04:39S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:40S		
Control 3 EC	0.100%	04:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:41S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312
10/31/2010

Badge No.: 312

Date: 10/31/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00433 Calib. Date: 08/13/2010 Calib. No.: 00013
Certification File No.: 00434 Cert. Date: 08/13/2010 Cert. No.: 00008
Linearity File No.: 00435 Lin. Date: 08/13/2010 Lin. No.: 00008
Solution File No.: 00446 Soln. Date: 10/02/2010 Soln. No.: 00099
Sequential File No.: 00446 File Date: 10/02/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0172

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:57D		
Control 1 EC	0.099%	10:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:58D		
Control 2 EC	0.099%	10:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59D		
Control 3 EC	0.100%	10:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Joseph T. Baumgardner #312 10/02/2010

Badge No.: 312

Date: 10/02/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00433	Calib. Date: 08/13/2010
Certification File No.:	00434	Calib. No.: 00013
Linearity File No.:	00435	Cert. Date: 08/13/2010
Solution File No.:	00443	Cert. No.: 00008
Sequential File No.:	00443	Lin. Date: 08/13/2010
		Lin. No.: 00008
		Soln. Date: 09/08/2010
		Soln. No.: 00098
		File Date: 09/08/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0152

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:01D		
Control 1 EC	0.100%	08:01D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 2 EC	0.100%	08:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03D		
Control 3 EC	0.100%	08:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature:  #319

Badge No.: 319

Date: 09/08/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00382	Calib. Date: 02/18/2010
Certification File No.:	00383	Calib. No.: 00008
Linearity File No.:	00384	Cert. Date: 02/18/2010
Solution File No.:	00419	Cert. No.: 00007
Sequential File No.:	00419	Lin. Date: 02/18/2010
		Lin. No.: 00007
		Soln. Date: 07/15/2010
		Soln. No.: 00091
		File Date: 07/15/2010

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0135
Control Solution %: 0.100%		Expires: 01/15/2011
Solution Control Lot: 09A062		Bottle No.: 0162

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:07D		
Control 1 EC	0.101%	08:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 2 EC	0.099%	08:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09D		
Control 3 EC	0.099%	08:10D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 07/15/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00382 Calib. Date: 02/18/2010 Calib. No.: 00008
Certification File No.: 00383 Cert. Date: 02/18/2010 Cert. No.: 00007
Linearity File No.: 00384 Lin. Date: 02/18/2010 Lin. No.: 00007
Solution File No.: 00412 Soln. Date: 06/22/2010 Soln. No.: 00090
Sequential File No.: 00412 File Date: 06/22/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0154

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:32D		
Control 1 EC	0.100%	08:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:34D		
Control 2 EC	0.099%	08:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:35D		
Control 3 EC	0.100%	08:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 6/22/2010

Badge No.: 312

Date: 06/22/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00382 Calib. Date: 02/18/2010 Calib. No.: 00008
Certification File No.: 00383 Cert. Date: 02/18/2010 Cert. No.: 00007
Linearity File No.: 00384 Lin. Date: 02/18/2010 Lin. No.: 00007
Solution File No.: 00399 Soln. Date: 05/25/2010 Soln. No.: 00089
Sequential File No.: 00399 File Date: 05/25/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0167

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:52D		
Control 1 EC	0.101%	20:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	20:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:53D		
Control 2 EC	0.100%	20:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:54D		
Control 3 EC	0.100%	20:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 5/25/2010

Badge No.: 312

Date: 05/25/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00382	Calib. Date: 02/18/2010
Certification File No.:	00383	Calib. No.: 00008
Linearity File No.:	00384	Cert. Date: 02/18/2010
Solution File No.:	00398	Cert. No.: 00007
Sequential File No.:	00398	Lin. Date: 02/18/2010
		Lin. No.: 00007
		Soln. Date: 04/23/2010
		Soln. No.: 00088
		File Date: 04/23/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0153

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:12D		
Control 1 EC	0.100%	10:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:14D		
Control 2 EC	0.099%	10:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		
Control 3 EC	0.100%	10:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DIDWAP2-199₂₀₀

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: _____

Tpr. II [Signature] # 6027

Badge No.: 6027

Date: 04/23/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00382 Calib. Date: 02/18/2010 Calib. No.: 00008
Certification File No.: 00383 Cert. Date: 02/18/2010 Cert. No.: 00007
Linearity File No.: 00384 Lin. Date: 02/18/2010 Lin. No.: 00007
Solution File No.: 00397 Soln. Date: 04/07/2010 Soln. No.: 00087
Sequential File No.: 00397 File Date: 04/07/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0159

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:11D		
Control 1 EC	0.099%	08:11D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12D		
Control 2 EC	0.098%	08:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:13D		
Control 3 EC	0.098%	08:14D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:14D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

 319

Badge No.: 319

Date: 04/07/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00382 Calib. Date: 02/18/2010 Calib. No.: 00008
Certification File No.: 00383 Cert. Date: 02/18/2010 Cert. No.: 00007
Linearity File No.: 00384 Lin. Date: 02/18/2010 Lin. No.: 00007
Solution File No.: 00392 Soln. Date: 03/16/2010 Soln. No.: 00086
Sequential File No.: 00392 File Date: 03/16/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0163

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:37S		
Control 1 EC	0.100%	21:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	21:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:39S		
Control 2 EC	0.099%	21:39S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:39S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:40S		
Control 3 EC	0.100%	21:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 3/16/2010

Badge No.: 312

Date: 03/16/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00343	Calib. Date: 08/18/2009
Certification File No.:	00344	Calib. No.: 00007
Linearity File No.:	00345	Cert. Date: 08/18/2009
Solution File No.:	00380	Cert. No.: 00006
Sequential File No.:	00380	Lin. Date: 08/18/2009
		Lin. No.: 00006
		Soln. Date: 02/10/2010
		Soln. No.: 00084
		File Date: 02/10/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0173

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:16S		
Control 1 EC	0.100%	08:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17S		
Control 2 EC	0.100%	08:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19S		
Control 3 EC	0.100%	08:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

[Handwritten Signature] #319

Badge No.: 319

Date: 02/10/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C		Serial No.: ARXA-0067
Location: LONGPORT POLICE		
Calibration File No.: 00343	Calib. Date: 08/18/2009	Calib. No.: 00007
Certification File No.: 00344	Cert. Date: 08/18/2009	Cert. No.: 00006
Linearity File No.: 00345	Lin. Date: 08/18/2009	Lin. No.: 00006
Solution File No.: 00379	Soln. Date: 01/17/2010	Soln. No.: 00083
Sequential File No.: 00379	File Date: 01/17/2010	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %: 0.100%		Expires: 01/15/2011
Solution Control Lot: 09A062		Bottle No.: 0158

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:03S		
Control 1 EC	0.103%	08:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:04S		
Control 2 EC	0.100%	08:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:06S		
Control 3 EC	0.100%	08:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

JMS

#319

Badge No.: 319

Date: 01/17/2010

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00343	Calib. Date: 08/18/2009
Certification File No.:	00344	Cert. No.: 00007
Linearity File No.:	00345	Cert. Date: 08/18/2009
Solution File No.:	00377	Lin. Date: 08/18/2009
Sequential File No.:	00377	Lin. No.: 00006
		Soln. Date: 01/07/2010
		Soln. No.: 00082
		File Date: 01/07/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0155

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:26S		
Control 1 EC	0.102%	11:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:28S		
Control 2 EC	0.100%	11:28S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	11:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29S		
Control 3 EC	0.100%	11:30S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Joseph T. Baumgardner

Joseph T. Baumgardner # 312 1/7/2010

Badge No.: 312

Date: 01/07/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 Calib. Date: 08/18/2009 Calib. No.: 00007
Certification File No.: 00344 Cert. Date: 08/18/2009 Cert. No.: 00006
Linearity File No.: 00345 Lin. Date: 08/18/2009 Lin. No.: 00006
Solution File No.: 00372 Soln. Date: 12/13/2009 Soln. No.: 00081
Sequential File No.: 00372 File Date: 12/13/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0168

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:07S		
Control 1 EC	0.100%	04:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:08S		
Control 2 EC	0.100%	04:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:09S		
Control 3 EC	0.100%	04:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

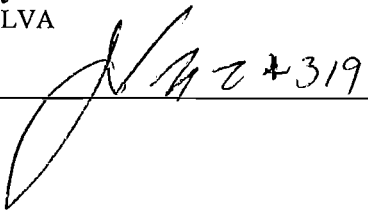

Badge No.: 319

Date: 12/13/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00343	Calib. Date: 08/18/2009
Certification File No.:	00344	Calib. No.: 00007
Linearity File No.:	00345	Cert. Date: 08/18/2009
Solution File No.:	00370	Cert. No.: 00006
Sequential File No.:	00370	Lin. Date: 08/18/2009
		Lin. No.: 00006
		Soln. Date: 11/24/2009
		Soln. No.: 00080
		File Date: 11/24/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %:	0.100%		Expires: 01/15/2011
Solution Control Lot:	09A062		Bottle No.: 0169

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:55S		
Control 1 EC	0.100%	17:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	17:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:57S		
Control 2 EC	0.099%	17:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:58S		
Control 3 EC	0.099%	17:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature: Joseph T. Baumgardner #312 11/24/09

Badge No.: 312

Date: 11/24/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE	Calib. Date:	08/18/2009
Calibration File No.:	00343	Calib. No.:	00007
Certification File No.:	00344	Cert. Date:	08/18/2009
Linearity File No.:	00345	Lin. Date:	08/18/2009
Solution File No.:	00365	Soln. Date:	10/30/2009
Sequential File No.:	00365	File Date:	10/30/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0154
Solution Control Lot:	09A062	Expires:	01/15/2011
		Bottle No.:	0164

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:07S		
Control 1 EC	0.100%	04:07S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:08S		
Control 2 EC	0.099%	04:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:10S		
Control 3 EC	0.099%	04:10S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

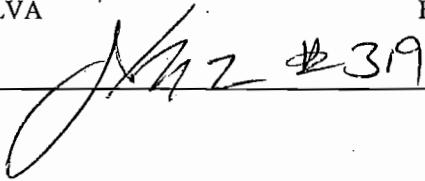

Badge No.: 319

Date: 10/30/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00343 Calib. Date: 08/18/2009 Calib. No.: 00007
Certification File No.: 00344 Cert. Date: 08/18/2009 Cert. No.: 00006
Linearity File No.: 00345 Lin. Date: 08/18/2009 Lin. No.: 00006
Solution File No.: 00361 Soln. Date: 10/05/2009 Soln. No.: 00077
Sequential File No.: 00361 File Date: 10/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 0175

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:37D		
Control 1 EC	0.101%	16:38D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:38D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:38D		
Control 2 EC	0.098%	16:39D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	16:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:40D		
Control 3 EC	0.099%	16:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

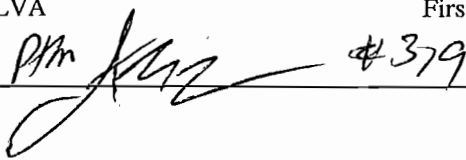

Badge No.: 319

Date: 10/05/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00343	Calib. Date: 08/18/2009
Certification File No.:	00344	Cert. No.: 00007
Linearity File No.:	00345	Cert. Date: 08/18/2009
Solution File No.:	00357	Lin. No.: 00006
Sequential File No.:	00357	Soln. Date: 09/12/2009
		Soln. No.: 00076
		File Date: 09/12/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0160

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:25D		
Control 1 EC	0.101%	00:26D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:26D		
Control 2 EC	0.100%	00:27D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	00:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:28D		
Control 3 EC	0.099%	00:28D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:28D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:29D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 09/12/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00343	Calib. Date: 08/18/2009
Certification File No.:	00344	Calib. No.: 00007
Linearity File No.:	00345	Cert. Date: 08/18/2009
Solution File No.:	00356	Cert. No.: 00006
Sequential File No.:	00356	Lin. Date: 08/18/2009
		Lin. No.: 00006
		Soln. Date: 09/11/2009
		Soln. No.: 00075
		File Date: 09/11/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	09A062	Expires: 01/15/2011
		Bottle No.: 0165

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:08D		
Control 1 EC	0.101%	20:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	20:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:10D		
Control 2 EC	0.100%	20:10D	34.0°C	AMBIENT AIR CHECK ERR
Control 2 IR	-.---%	20:10D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	0.030%	20:11D		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 09/11/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00284	Calib. Date: 02/23/2009
Certification File No.:	00285	Calib. No.: 00006
Linearity File No.:	00286	Cert. Date: 02/23/2009
Solution File No.:	00341	Cert. No.: 00005
Sequential File No.:	00341	Lin. Date: 02/23/2009
		Lin. No.: 00005
		Soln. Date: 08/14/2009
		Soln. No.: 00073
		File Date: 08/14/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %: 0.100%		Expires: 02/13/2010
Solution Control Lot: 08B050		Bottle No.: 0516

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:40D		
Control 1 EC	0.101%	12:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	12:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:41D		
Control 2 EC	0.100%	12:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43D		
Control 3 EC	0.099%	12:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____

Badge No.: 319

Date: 08/14/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00284	Calib. Date: 02/23/2009
Certification File No.:	00285	Calib. No.: 00006
Linearity File No.:	00286	Cert. Date: 02/23/2009
Solution File No.:	00330	Cert. No.: 00005
Sequential File No.:	00330	Lin. Date: 02/23/2009
		Lin. No.: 00005
		Soln. Date: 07/14/2009
		Soln. No.: 00071
		File Date: 07/14/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXC S3-0154
Control Solution %:	0.100%		Expires: 02/13/2010
Solution Control Lot:	08B050		Bottle No.: 0513

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:15D		
Control 1 EC	0.099%	11:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 2 EC	0.099%	11:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18D		
Control 3 EC	0.099%	11:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 7/14/09

Badge No.: 312

Date: 07/14/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00284 Calib. Date: 02/23/2009 Calib. No.: 00006
Certification File No.: 00285 Cert. Date: 02/23/2009 Cert. No.: 00005
Linearity File No.: 00286 Lin. Date: 02/23/2009 Lin. No.: 00005
Solution File No.: 00310 Soln. Date: 06/18/2009 Soln. No.: 00070
Sequential File No.: 00310 File Date: 06/18/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0154
Control Solution %: 0.100% Expires: 02/13/2010
Solution Control Lot: 08B050 Bottle No.: 0345

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:01D		
Control 1 EC	0.101%	05:01D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	05:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:02D		
Control 2 EC	0.100%	05:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:03D		
Control 3 EC	0.100%	05:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	05:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 6/18/09

Badge No.: 312

Date: 06/18/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0067
Location:	LONGPORT POLICE	Calib. Date:	02/23/2009
Calibration File No.:	00284	Cert. No.:	00006
Certification File No.:	00285	Cert. Date:	02/23/2009
Linearity File No.:	00286	Lin. Date:	02/23/2009
Solution File No.:	00307	Soln. No.:	00005
Sequential File No.:	00307	Soln. Date:	06/06/2009
		File Date:	06/06/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0154
Solution Control Lot:	08B050	Expires:	02/13/2010
		Bottle No.:	0506

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:44D		
Control 1 EC	0.100%	08:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:45D		
Control 2 EC	0.099%	08:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46D		
Control 3 EC	0.099%	08:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 06/06/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00284	Calib. Date: 02/23/2009
Certification File No.:	00285	Calib. No.: 00006
Linearity File No.:	00286	Cert. Date: 02/23/2009
Solution File No.:	00302	Cert. No.: 00005
Sequential File No.:	00302	Lin. Date: 02/23/2009
		Lin. No.: 00005
		Soln. Date: 05/19/2009
		Soln. No.: 00068
		File Date: 05/19/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 0522

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:01D		
Control 1 EC	0.102%	10:02D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:02D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03D		
Control 2 EC	0.101%	10:03D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:03D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04D		
Control 3 EC	0.101%	10:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWAP2-177js

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *TP: F J Sullivan*

Badge No.: 5103

Date: 05/19/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00284	Calib. Date: 02/23/2009
Certification File No.:	00285	Calib. No.: 00006
Linearity File No.:	00286	Cert. Date: 02/23/2009
Solution File No.:	00299	Cert. No.: 00005
Sequential File No.:	00299	Lin. Date: 02/23/2009
		Lin. No.: 00005
		Soln. Date: 05/11/2009
		Soln. No.: 00067
		File Date: 05/11/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0135
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 0521

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:50D		
Control 1 EC	0.101%	10:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52D		
Control 2 EC	0.100%	10:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:53D		
Control 3 EC	0.100%	10:54D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 5/11/09

Badge No.: 312

Date: 05/11/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0067
Location: LONGPORT POLICE
Calibration File No.: 00256 Calib. Date: 08/26/2008 Calib. No.: 00005
Certification File No.: 00257 Cert. Date: 08/26/2008 Cert. No.: 00004
Linearity File No.: 00258 Lin. Date: 08/26/2008 Lin. No.: 00004
Solution File No.: 00278 Soln. Date: 01/21/2009 Soln. No.: 00062
Sequential File No.: 00278 File Date: 01/21/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0135
Control Solution %: 0.100% Expires: 02/13/2010
Solution Control Lot: 08B050 Bottle No.: 0519

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:28S		
Control 1 EC	0.103%	14:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:29S		
Control 2 EC	0.100%	14:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:31S		
Control 3 EC	0.100%	14:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature probe serial number: DDWAP2-19935

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *Francis J Sullivan #5103*

Badge No.: 5103

Date: 01/21/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00256	Calib. Date: 08/26/2008
Certification File No.:	00257	Calib. No.: 00005
Linearity File No.:	00258	Cert. Date: 08/26/2008
Solution File No.:	00266	Cert. No.: 00004
Sequential File No.:	00266	Lin. Date: 08/26/2008
		Lin. No.: 00004
		Soln. Date: 11/08/2008
		Soln. No.: 00058
		File Date: 11/08/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 0520

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:45S		
Control 1 EC	0.099%	00:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:47S		
Control 2 EC	0.099%	00:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	00:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:48S		
Control 3 EC	0.099%	00:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:49S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SILVA

First Name: JAMES

MI: F

Signature: _____



Badge No.: 319

Date: 11/08/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0067
Location:	LONGPORT POLICE	
Calibration File No.:	00211	Calib. Date: 03/28/2008
Certification File No.:	00212	Calib. No.: 00004
Linearity File No.:	00213	Cert. Date: 03/28/2008
Solution File No.:	00247	Cert. No.: 00003
Sequential File No.:	00247	Lin. Date: 03/28/2008
		Lin. No.: 00003
		Soln. Date: 08/15/2008
		Soln. No.: 00052
		File Date: 08/15/2008

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0154
Solution Control Lot:	08B050	Expires: 02/13/2010
		Bottle No.: 0509

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:43D		
Control 1 EC	0.100%	09:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		
Control 2 EC	0.100%	09:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		
Control 3 EC	0.099%	09:46D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BAUMGARDNER

First Name: JOSEPH

MI: T

Signature:

Joseph T. Baumgardner #312 8/15/08

Badge No.: 312

Date: 08/15/2008