

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00004	Calib. Date:	04/13/2006
Certification File No.:	00005	Cert. Date:	04/13/2006
Linearity File No.:	00006	Lin. Date:	04/13/2006
Solution File No.:	00007	Soln. Date:	04/13/2006
Sequential File No.:	00007	File Date:	04/13/2006
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0004
Solution Control Lot:	06B023	Expires:	02/10/2008
		Bottle No.:	0364

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:13D		
Control 1 EC	0.099%	15:14D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:14D		
Control 2 EC	0.098%	15:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:16D		
Control 3 EC	0.098%	15:16D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJFZ-156 *ams*

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: *TPZ I Adam N Stanks #5403*

Badge No.: 5403

Date: 04/13/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00012	Cert. No.: 00001
Sequential File No.:	00012	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 05/06/2006
		Soln. No.: 00003
		File Date: 05/06/2006

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXA S3-0004
Control Solution %: 0.100%		Expires: 02/10/2008
Solution Control Lot: 06B023		Bottle No.: 0320

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:04D		
Control 1 EC	0.097%	19:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:05D		
Control 2 EC	0.097%	19:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	19:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:07D		
Control 3 EC	0.097%	19:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	19:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 05/06/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00014	Cert. No.: 00001
Sequential File No.:	00014	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 06/03/2006
		Soln. No.: 00004
		File Date: 06/03/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0004
Solution Control Lot:	06B023	Expires: 02/10/2008
		Bottle No.: 0317

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:06D		
Control 1 EC	0.095%	08:06D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07D		
Control 2 EC	0.096%	08:08D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	08:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 3 EC	0.096%	08:09D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Badge No.: 629

Date: 06/03/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00018	Cert. No.: 00001
Sequential File No.:	00018	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 06/24/2006
		Soln. No.: 00005
		File Date: 06/24/2006

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXA S3-0004
Control Solution %: 0.100%		Expires: 03/16/2008
Solution Control Lot: 06C030		Bottle No.: 0377

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:06D		
Control 1 EC	0.096%	12:07D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	12:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07D		
Control 2 EC	0.096%	12:08D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	12:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:09D		
Control 3 EC	0.097%	12:09D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	12:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

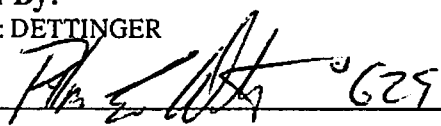

Badge No.: 629

Date: 06/24/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00025	Cert. No.: 00001
Sequential File No.:	00025	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 07/19/2006
		Soln. No.: 00007
		File Date: 07/19/2006
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0004
Solution Control Lot:	06B023	Expires: 02/10/2008
		Bottle No.: 0322

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:22D		
Control 1 EC	0.098%	03:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	03:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:23D		
Control 2 EC	0.098%	03:24D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:25D		
Control 3 EC	0.098%	03:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	03:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:26D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 07/19/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00029	Cert. No.: 00001
Sequential File No.:	00029	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 08/12/2006
		Soln. No.: 00008
		File Date: 08/12/2006

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0004
Control Solution %:	0.100%		Expires: 02/10/2008
Solution Control Lot:	06B023		Bottle No.: 0311

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:51D		
Control 1 EC	0.097%	12:51D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	12:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:52D		
Control 2 EC	0.097%	12:53D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	12:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:53D		
Control 3 EC	0.097%	12:54D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	12:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Badge No.: 629

Date: 08/12/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00034	Cert. No.: 00001
Sequential File No.:	00034	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 09/08/2006
		Soln. No.: 00009
		File Date: 09/08/2006

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0004
Control Solution %:	0.100%		Expires: 02/10/2008
Solution Control Lot:	06B023		Bottle No.: 0316

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:24D		
Control 1 EC	0.098%	05:24D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:25D		
Control 2 EC	0.097%	05:25D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	05:25D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:26D		
Control 3 EC	0.097%	05:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Badge No.: 629

Date: 09/08/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00004	Calib. Date:	04/13/2006
Certification File No.:	00005	Cert. No.:	00002
Linearity File No.:	00006	Cert. Date:	04/13/2006
Solution File No.:	00036	Lin. No.:	00001
Sequential File No.:	00036	Lin. Date:	04/13/2006
		Soln. No.:	00011
		Soln. Date:	10/07/2006
		File Date:	10/07/2006
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0004
Solution Control Lot:	06C027	Expires:	03/03/2008
		Bottle No.:	0487

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:09D		
Control 1 EC	0.098%	11:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10D		
Control 2 EC	0.098%	11:11D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12D		
Control 3 EC	0.097%	11:12D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Badge No.: 629

Date: 10/07/2006

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00004 **Calib. Date:** 04/13/2006 **Calib. No.:** 00002
Certification File No.: 00005 **Cert. Date:** 04/13/2006 **Cert. No.:** 00001
Linearity File No.: 00006 **Lin. Date:** 04/13/2006 **Lin. No.:** 00001
Solution File No.: 00039 **Soln. Date:** 11/03/2006 **Soln. No.:** 00012
Sequential File No.: 00039 **File Date:** 11/03/2006

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDXA S3-0005
Control Solution %: 0.100% **Expires:** 03/03/2008
Solution Control Lot: 06C027 **Bottle No.:** 0491

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:19S		
Control 1 EC	0.098%	12:19S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:20S		
Control 2 EC	0.098%	12:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	12:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		
Control 3 EC	0.098%	12:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJFZ - 157 WNS

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: TPR I Adam N. Stanks #5403

Badge No.: 5403

Date: 11/03/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00040	Cert. No.: 00001
Sequential File No.:	00040	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 12/01/2006
		Soln. No.: 00013
		File Date: 12/01/2006

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 03/03/2008
Solution Control Lot:	06C027		Bottle No.: 0490

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:24S		
Control 1 EC	0.099%	10:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:25S		
Control 2 EC	0.097%	10:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26S		
Control 3 EC	0.097%	10:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Eric Dettinger 629

Badge No.: 629

Date: 12/01/2006

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00046	Cert. No.: 00001
Sequential File No.:	00046	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 12/29/2006
		Soln. No.: 00014
		File Date: 12/29/2006

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 03/03/2008
Solution Control Lot:	06C027		Bottle No.: 0499

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:34S		
Control 1 EC	0.100%	19:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	19:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:35S		
Control 2 EC	0.099%	19:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:37S		
Control 3 EC	0.099%	19:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Phm. E. Dettinger 629

Badge No.: 629

Date: 12/29/2006

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00004	Calib. Date:	04/13/2006
Certification File No.:	00005	Cert. No.:	00002
Linearity File No.:	00006	Cert. Date:	04/13/2006
Solution File No.:	00051	Lin. Date:	04/13/2006
Sequential File No.:	00051	Lin. No.:	00001
		Soln. Date:	01/22/2007
		Soln. No.:	00015
		File Date:	01/22/2007

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0005
Control Solution %:	0.100%			Expires:	03/03/2008
Solution Control Lot:	06C027			Bottle No.:	0483

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:47S		
Control 1 EC	0.098%	11:48S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48S		
Control 2 EC	0.098%	11:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50S		
Control 3 EC	0.098%	11:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 01/22/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00004	Calib. Date: 04/13/2006
Certification File No.:	00005	Calib. No.: 00002
Linearity File No.:	00006	Cert. Date: 04/13/2006
Solution File No.:	00054	Cert. No.: 00001
Sequential File No.:	00054	Lin. Date: 04/13/2006
		Lin. No.: 00001
		Soln. Date: 02/20/2007
		Soln. No.: 00017
		File Date: 02/20/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	06C027	Expires: 03/03/2008
		Bottle No.: 0486

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:10S		
Control 1 EC	0.099%	15:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:11S		
Control 2 EC	0.098%	15:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	15:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:12S		
Control 3 EC	0.098%	15:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	15:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 02/20/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00058	Calib. Date: 03/07/2007
Certification File No.:	00059	Calib. No.: 00003
Linearity File No.:	00060	Cert. Date: 03/07/2007
Solution File No.:	00064	Cert. No.: 00002
Sequential File No.:	00064	Lin. Date: 03/07/2007
		Lin. No.: 00002
		Soln. Date: 03/22/2007
		Soln. No.: 00020
		File Date: 03/22/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	06C027	Expires: 03/03/2008
		Bottle No.: 0478

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:03S		
Control 1 EC	0.098%	16:04S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:04S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:04S		
Control 2 EC	0.098%	16:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	16:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:06S		
Control 3 EC	0.098%	16:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	16:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Badge No.: 629

Date: 03/22/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00058	Calib. Date: 03/07/2007
Certification File No.:	00059	Cert. No.: 00003
Linearity File No.:	00060	Cert. Date: 03/07/2007
Solution File No.:	00068	Lin. No.: 00002
Sequential File No.:	00068	Soln. Date: 04/15/2007
		Soln. No.: 00022
		File Date: 04/15/2007

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 03/03/2008
Solution Control Lot:	06C027		Bottle No.: 0481

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:00D		
Control 1 EC	0.097%	21:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	21:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:01D		
Control 2 EC	0.097%	21:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	21:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:02D		
Control 3 EC	0.097%	21:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	21:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 04/15/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00058	Calib. No.: 00003
Certification File No.:	00059	Cert. No.: 00002
Linearity File No.:	00060	Lin. No.: 00002
Solution File No.:	00074	Soln. No.: 00026
Sequential File No.:	00074	File Date: 05/15/2007

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 03/03/2008
Solution Control Lot:	06C027		Bottle No.: 0498

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:23D		
Control 1 EC	0.095%	14:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	14:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:24D		
Control 2 EC	0.095%	14:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	14:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:25D		
Control 3 EC	0.095%	14:26D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.095%	14:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 05/15/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00081	Calib. Date:	05/31/2007
Certification File No.:	00082	Cert. Date:	05/31/2007
Linearity File No.:	00083	Lin. Date:	05/31/2007
Solution File No.:	00084	Soln. Date:	05/31/2007
Sequential File No.:	00084	File Date:	05/31/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0005
Solution Control Lot:	06C027	Expires:	03/03/2008
		Bottle No.:	0477

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:47D		
Control 1 EC	0.102%	11:48D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:48D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48D		
Control 2 EC	0.102%	11:49D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:49D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50D		
Control 3 EC	0.102%	11:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJFZ-157 *ans*

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: *TPR I Adam N Stanks #5403*

Badge No.: 5403

Date: 05/31/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Calib. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00091	Cert. No.: 00003
Sequential File No.:	00091	Lin. Date: 05/31/2007
		Lin. No.: 00003
		Soln. No.: 00030
		File Date: 06/24/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	06B023	Expires: 02/10/2008
		Bottle No.: 0312

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:09D		
Control 1 EC	0.102%	20:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	20:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:10D		
Control 2 EC	0.101%	20:10D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:11D		
Control 3 EC	0.101%	20:11D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 06/24/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Cert. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00100	Lin. No.: 00003
Sequential File No.:	00100	Lin. Date: 05/31/2007
		Soln. No.: 00032
		Soln. Date: 07/27/2007
		File Date: 07/27/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	06C027	Expires: 03/03/2008
		Bottle No.: 0480

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:27D		
Control 1 EC	0.101%	09:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		
Control 2 EC	0.101%	09:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29D		
Control 3 EC	0.100%	09:30D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 07/27/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	Calib. No.:	00005
Calibration File No.:	00081	Calib. Date:	05/31/2007
Certification File No.:	00082	Cert. Date:	05/31/2007
Linearity File No.:	00083	Lin. Date:	05/31/2007
Solution File No.:	00113	Soln. Date:	08/24/2007
Sequential File No.:	00113	File Date:	08/24/2007
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0005
Solution Control Lot:	06C027	Expires:	03/03/2008
		Bottle No.:	0482

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:31D		
Control 1 EC	0.100%	20:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:32D		
Control 2 EC	0.100%	20:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:33D		
Control 3 EC	0.100%	20:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 08/24/2007

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00081 Calib. Date: 05/31/2007 Calib. No.: 00005
Certification File No.: 00082 Cert. Date: 05/31/2007 Cert. No.: 00003
Linearity File No.: 00083 Lin. Date: 05/31/2007 Lin. No.: 00003
Solution File No.: 00124 Soln. Date: 08/28/2007 Soln. No.: 00035
Sequential File No.: 00124 File Date: 08/28/2007

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 04/24/2009
Solution Control Lot: 07B046 Bottle No.: 0281

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:18D		
Control 1 EC	0.100%	21:18D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	21:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:19D		
Control 2 EC	0.100%	21:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:20D		
Control 3 EC	0.100%	21:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	21:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 08/28/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Calib. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00129	Cert. No.: 00003
Sequential File No.:	00129	Lin. Date: 05/31/2007
		Lin. No.: 00003
		Soln. Date: 09/14/2007
		Soln. No.: 00036
		File Date: 09/14/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0292

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:10D		
Control 1 EC	0.100%	19:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	19:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:11D		
Control 2 EC	0.099%	19:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:12D		
Control 3 EC	0.099%	19:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	19:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

Eric Dettinger 629

Badge No.: 629

Date: 09/14/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. No.: 00005
Certification File No.:	00082	Cert. No.: 00003
Linearity File No.:	00083	Lin. No.: 00003
Solution File No.:	00137	Soln. No.: 00037
Sequential File No.:	00137	
	Calib. Date: 05/31/2007	
	Cert. Date: 05/31/2007	
	Lin. Date: 05/31/2007	
	Soln. Date: 10/15/2007	
	File Date: 10/15/2007	
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0276

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:45D		
Control 1 EC	0.101%	20:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	20:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:46D		
Control 2 EC	0.100%	20:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:47D		
Control 3 EC	0.100%	20:48D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:49D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 10/15/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C		Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00081	Calib. Date: 05/31/2007	Calib. No.: 00005
Certification File No.:	00082	Cert. Date: 05/31/2007	Cert. No.: 00003
Linearity File No.:	00083	Lin. Date: 05/31/2007	Lin. No.: 00003
Solution File No.:	00146	Soln. Date: 11/20/2007	Soln. No.: 00039
Sequential File No.:	00146	File Date: 11/20/2007	

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0005
Control Solution %:	0.100%			Expires:	04/24/2009
Solution Control Lot:	07B046			Bottle No.:	0287

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:16S		
Control 1 EC	0.102%	13:16S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:16S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17S		
Control 2 EC	0.101%	13:18S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:18S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18S		
Control 3 EC	0.101%	13:19S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.102%	13:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 11/20/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Cert. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00147	Lin. No.: 00003
Sequential File No.:	00147	Soln. Date: 11/20/2007
		Lin. No.: 00003
		Soln. No.: 00040
		File Date: 11/20/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0280

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:56S		
Control 1 EC	0.102%	15:56S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	15:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:57S		
Control 2 EC	0.102%	15:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:58S		
Control 3 EC	0.101%	15:59S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:59S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJFZ-157 *ams*

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: *TPR I Adam N. Stanks # 5403*

Badge No.: 5403

Date: 11/20/2007

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Cert. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00156	Lin. No.: 00003
Sequential File No.:	00156	Lin. Date: 05/31/2007
		Soln. No.: 00041
		Soln. Date: 12/19/2007
		File Date: 12/19/2007
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0278

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:30S		
Control 1 EC	0.103%	09:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	09:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 2 EC	0.102%	09:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32S		
Control 3 EC	0.101%	09:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

M1: F

Signature: Sgt. E. Dettinger 629

Badge No.: 629

Date: 12/19/2007

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Calib. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00166	Cert. No.: 00003
Sequential File No.:	00166	Lin. Date: 05/31/2007
		Lin. No.: 00003
		Soln. Date: 01/17/2008
		Soln. No.: 00042
		File Date: 01/17/2008

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0005
Control Solution %:	0.100%			Expires:	04/24/2009
Solution Control Lot:	07B046			Bottle No.:	0279

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:11S		
Control 1 EC	0.100%	08:12S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12S		
Control 2 EC	0.101%	08:13S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:14S		
Control 3 EC	0.100%	08:14S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 01/17/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Cert. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00168	Lin. No.: 00003
Sequential File No.:	00168	Soln. Date: 01/31/2008
		Soln. No.: 00043
		File Date: 01/31/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0285

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:03S		
Control 1 EC	0.101%	09:03S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04S		
Control 2 EC	0.101%	09:04S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	09:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05S		
Control 3 EC	0.101%	09:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 01/31/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00081	Calib. Date: 05/31/2007
Certification File No.:	00082	Calib. No.: 00005
Linearity File No.:	00083	Cert. Date: 05/31/2007
Solution File No.:	00170	Cert. No.: 00003
Sequential File No.:	00170	Lin. Date: 05/31/2007
		Lin. No.: 00003
		Soln. Date: 02/26/2008
		Soln. No.: 00044
		File Date: 02/26/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0284

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:49S		
Control 1 EC	0.100%	20:50S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:51S		
Control 2 EC	0.100%	20:51S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:51S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:52S		
Control 3 EC	0.101%	20:53S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 02/26/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00081 Calib. Date: 05/31/2007 Calib. No.: 00005
Certification File No.: 00082 Cert. Date: 05/31/2007 Cert. No.: 00003
Linearity File No.: 00083 Lin. Date: 05/31/2007 Lin. No.: 00003
Solution File No.: 00173 Soln. Date: 03/26/2008 Soln. No.: 00045
Sequential File No.: 00173 File Date: 03/26/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 04/24/2009
Solution Control Lot: 07B046 Bottle No.: 0283

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:33S		
Control 1 EC	0.100%	07:33S	33.8°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:33S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:34S		
Control 2 EC	0.100%	07:34S	33.8°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:34S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:35S		
Control 3 EC	0.100%	07:36S	33.8°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:36S	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:36S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 03/26/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00178	Calib. Date: 04/07/2008
Certification File No.:	00179	Calib. No.: 00006
Linearity File No.:	00180	Cert. Date: 04/07/2008
Solution File No.:	00192	Cert. No.: 00004
Sequential File No.:	00192	Lin. Date: 04/07/2008
		Lin. No.: 00004
		Soln. Date: 05/23/2008
		Soln. No.: 00048
		File Date: 05/23/2008

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0297

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:44D		
Control 1 EC	0.101%	14:44D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:45D		
Control 2 EC	0.100%	14:45D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:46D		
Control 3 EC	0.100%	14:47D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NEWMAN

First Name: PAUL

MI: S

Signature: _____

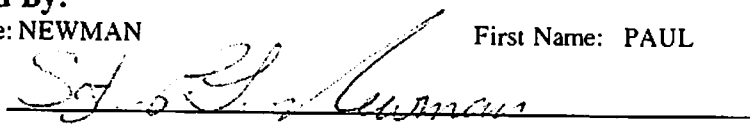

Badge No.: 619

Date: 05/23/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00178	Calib. Date: 04/07/2008
Certification File No.:	00179	Calib. No.: 00006
Linearity File No.:	00180	Cert. Date: 04/07/2008
Solution File No.:	00203	Cert. No.: 00004
Sequential File No.:	00203	Lin. Date: 04/07/2008
		Lin. No.: 00004
		Soln. Date: 06/17/2008
		Soln. No.: 00049
		File Date: 06/17/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0290

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:35D		
Control 1 EC	0.099%	20:36D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:37D		
Control 2 EC	0.097%	20:37D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:37D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:38D		
Control 3 EC	0.097%	20:38D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:39D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 06/17/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00212	Calib. Date: 08/04/2008
Certification File No.:	00213	Calib. No.: 00009
Linearity File No.:	00214	Cert. Date: 08/04/2008
Solution File No.:	00216	Cert. No.: 00005
Sequential File No.:	00216	Lin. Date: 08/04/2008
		Lin. No.: 00005
		Soln. Date: 08/22/2008
		Soln. No.: 00052
		File Date: 08/22/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0300

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:55D		
Control 1 EC	0.099%	09:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56D		
Control 2 EC	0.098%	09:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57D		
Control 3 EC	0.098%	09:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWJP 3 - 157, 2nd

Changed By:

Last Name: DELLANOCE

First Name: JOSEPH

MI: S

Signature: Tr. JSA #6027

Badge No.: 6027

Date: 08/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00212	Calib. Date: 08/04/2008
Certification File No.:	00213	Cert. No.: 00009
Linearity File No.:	00214	Cert. Date: 08/04/2008
Solution File No.:	00229	Lin. No.: 00005
Sequential File No.:	00229	Lin. Date: 08/04/2008
		Soln. No.: 00054
		Soln. Date: 09/15/2008
		File Date: 09/15/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0289

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:15D		
Control 1 EC	0.098%	07:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:16D		
Control 2 EC	0.098%	07:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:17D		
Control 3 EC	0.098%	07:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

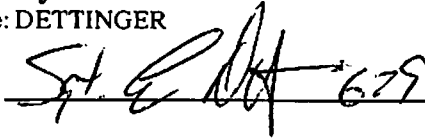

Badge No.: 629

Date: 09/15/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00212	Calib. Date: 08/04/2008
Certification File No.:	00213	Calib. No.: 00009
Linearity File No.:	00214	Cert. Date: 08/04/2008
Solution File No.:	00232	Cert. No.: 00005
Sequential File No.:	00232	Lin. Date: 08/04/2008
		Lin. No.: 00005
		Soln. Date: 09/24/2008
		Soln. No.: 00055
		File Date: 09/24/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0291

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:32D		
Control 1 EC	0.098%	03:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	03:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:33D		
Control 2 EC	0.097%	03:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:34D		
Control 3 EC	0.098%	03:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

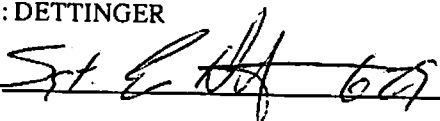

Badge No.: 629

Date: 09/24/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00212	Calib. Date: 08/04/2008
Certification File No.:	00213	Calib. No.: 00009
Linearity File No.:	00214	Cert. Date: 08/04/2008
Solution File No.:	00241	Cert. No.: 00005
Sequential File No.:	00241	Lin. Date: 08/04/2008
		Lin. No.: 00005
		Soln. Date: 10/22/2008
		Soln. No.: 00057
		File Date: 10/22/2008

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 04/29/2009
Solution Control Lot:	07B046		Bottle No.: 0294

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:04D		
Control 1 EC	0.102%	14:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	14:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 2 EC	0.100%	14:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:06D		
Control 3 EC	0.100%	14:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

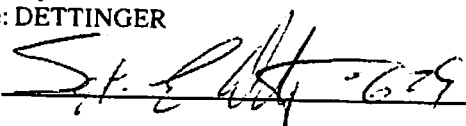

Badge No.: 629

Date: 10/22/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00212	Calib. Date: 08/04/2008
Certification File No.:	00213	Cert. No.: 00009
Linearity File No.:	00214	Cert. Date: 08/04/2008
Solution File No.:	00247	Lin. No.: 00005
Sequential File No.:	00247	Soln. No.: 00058
		File Date: 11/18/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0295

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:13S		
Control 1 EC	0.100%	21:14S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:14S		
Control 2 EC	0.098%	21:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	21:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:16S		
Control 3 EC	0.098%	21:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:17S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 11/18/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	Calib. No.:	00009
Calibration File No.:	00212	Cert. Date:	08/04/2008
Certification File No.:	00213	Lin. Date:	08/04/2008
Linearity File No.:	00214	Soln. Date:	12/14/2008
Solution File No.:	00259	File Date:	12/14/2008
Sequential File No.:	00259		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0005
Control Solution %:	0.100%			Expires:	04/24/2009
Solution Control Lot:	07B046			Bottle No.:	0293

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:32S		
Control 1 EC	0.099%	07:33S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:33S		
Control 2 EC	0.098%	07:34S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:35S		
Control 3 EC	0.098%	07:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:36S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 12/14/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00266	Calib. Date: 01/09/2009
Certification File No.:	00267	Calib. No.: 00012
Linearity File No.:	00268	Cert. Date: 01/09/2009
Solution File No.:	00272	Cert. No.: 00006
Sequential File No.:	00272	Lin. Date: 01/09/2009
		Lin. No.: 00006
		Soln. Date: 01/24/2009
		Soln. No.: 00064
		File Date: 01/24/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0005
Solution Control Lot:	07B046	Expires: 04/24/2009
		Bottle No.: 0298

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:52S		
Control 1 EC	0.101%	20:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:54S		
Control 2 EC	0.101%	20:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:55S		
Control 3 EC	0.101%	20:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:57S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 01/24/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0022
Location:	NORTHFIELD POLICE DEPT.	
Calibration File No.:	00266	Calib. No.: 00012
Certification File No.:	00267	Cert. No.: 00006
Linearity File No.:	00268	Lin. No.: 00006
Solution File No.:	00274	Soln. No.: 00065
Sequential File No.:	00274	File Date: 02/21/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDXA S3-0005
Control Solution %:	0.100%		Expires: 04/24/2009
Solution Control Lot:	07B046		Bottle No.: 0296

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:27S		
Control 1 EC	0.101%	11:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	11:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:29S		
Control 2 EC	0.100%	11:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:30S		
Control 3 EC	0.100%	11:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 02/21/2009

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0022
Location:	NORTHFIELD POLICE DEPT.		
Calibration File No.:	00266	Calib. Date:	01/09/2009
Certification File No.:	00267	Cert. Date:	01/09/2009
Linearity File No.:	00268	Lin. Date:	01/09/2009
Solution File No.:	00285	Soln. Date:	04/23/2009
Sequential File No.:	00285	File Date:	04/23/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0005
Solution Control Lot:	08L061	Expires:	12/01/2010
		Bottle No.:	0464

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:18D		
Control 1 EC	0.100%	08:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19D		
Control 2 EC	0.100%	08:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:21D		
Control 3 EC	0.100%	08:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____



Badge No.: 629

Date: 04/23/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00266 Calib. Date: 01/09/2009 Calib. No.: 00012
Certification File No.: 00267 Cert. Date: 01/09/2009 Cert. No.: 00006
Linearity File No.: 00268 Lin. Date: 01/09/2009 Lin. No.: 00006
Solution File No.: 00289 Soln. Date: 04/28/2009 Soln. No.: 00068
Sequential File No.: 00289 File Date: 04/28/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 12/01/2010
Solution Control Lot: 08L061 Bottle No.: 0454

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:28D		
Control 1 EC	0.098%	02:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:29D		
Control 2 EC	0.098%	02:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	02:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:31D		
Control 3 EC	0.098%	02:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: 

Badge No.: 629

Date: 04/28/2009

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0022
Location: NORTHFIELD POLICE DEPT.
Calibration File No.: 00266 Calib. Date: 01/09/2009 Calib. No.: 00012
Certification File No.: 00267 Cert. Date: 01/09/2009 Cert. No.: 00006
Linearity File No.: 00268 Lin. Date: 01/09/2009 Lin. No.: 00006
Solution File No.: 00291 Soln. Date: 05/01/2009 Soln. No.: 00069
Sequential File No.: 00291 File Date: 05/01/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0005
Control Solution %: 0.100% Expires: 12/01/2010
Solution Control Lot: 08L061 Bottle No.: 0453

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:17D		
Control 1 EC	0.100%	20:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18D		
Control 2 EC	0.098%	20:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:20D		
Control 3 EC	0.099%	20:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DETTINGER

First Name: ERIC

MI: F

Signature: _____

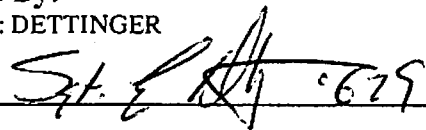

Badge No.: 629

Date: 05/01/2009